

D-7000 HPLC System Manager Report

Analyzed: 18.09.13 12:12

Reported: 18.09.13 14:36

Processed: 18.09.13 14:35

Data Path: C:\Win32App\HSM\samples\DATA\2271\

Processing Method: DAD2 Nucleodur C18ec

System(acquisition): DAD 2

Series:2271

Application: Samples

Vial Number: 2

Sample Name: mcnffs -lim

Vial Type: UNK

Injection from this vial: 1 of 1

Volume: 10,0 ul


Sample Description:

Absorbance Mode: NORMAL(2.0 AU)


Absorbance Scale: 0.800

Spectral Bandwidth: AUTO

Spectral Interval: 1600 ms

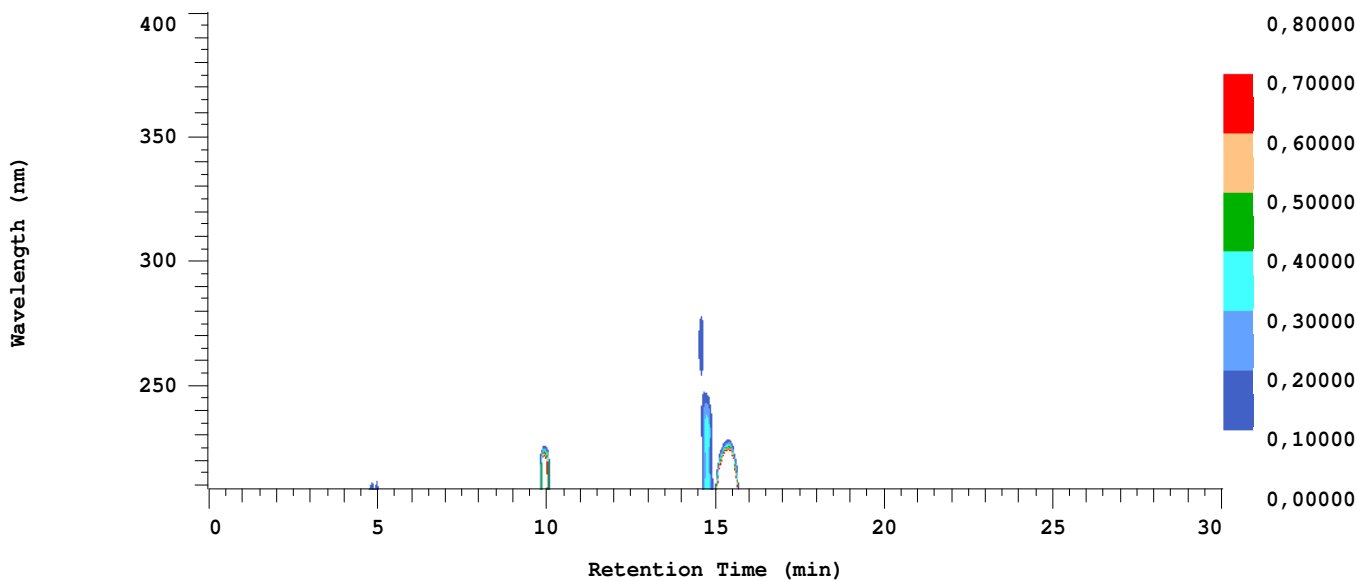

Chrom Type: Integrated Chromatogram, 209 to 400 nm

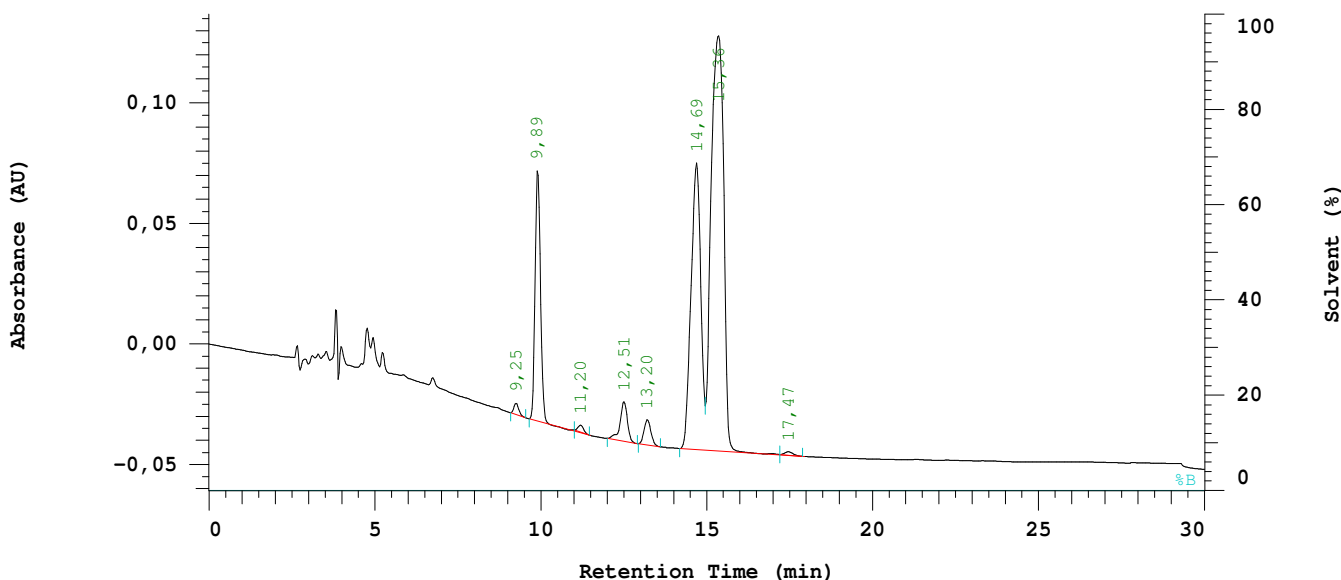

Acquisition Method: DAD2 Nucleodur C18ec

Column Type: MN Nucleodur 100-5 C18ec Developed by:

Pump A Type: L-7100

Solvent A: ACN

Solvent B: 0.1% TFA

Solvent C: Wasser20

Solvent D: 0

Method Description:

Chrom Type: Integrated Chromatogram, 209 to 400 nm

Peak Quantitation: AREA

Calculation Method: AREA%

No.	RT	Area	Conc 1	BC
1	9,25	24951	0,577	BB
2	9,89	591960	13,678	BB
3	11,20	18016	0,416	TBB
4	12,51	127985	2,957	BB
5	13,20	76050	1,757	BB
6	14,69	1204289	27,826	BV
7	15,36	2271934	52,494	VB
8	17,47	12773	0,295	TBB
		4327958	100,000	

Peak rejection level: 0

Channel 1 Noise: Not Measured
Channel 1 Drift: Not Measured

Configuration parameters:

Interface Module: D-7000	Gradient Mode: Low
Channel 1 Detector: L-7455	Channel 2 Detector: None
Column Oven: None	Autosampler: L-7250
Pump A: L-7100	Pump B: None
Number of Solvents pump A: 4	Number of Solvents pump B: 1
External Instrument Software: None	Column Name: MN Nucleodur 100-5 C18ec

Method Information:

Method Name: DAD2 Nucleodur C18ec	Developed by:
Description:	

Pump Setup:

Main Pump (A) Pressure Limit: 0 to 412 bar

Pump A (L-7100):

Solvent A: ACN	Solvent B: 0.1% TFA
Solvent C: Wasser20	Solvent D: 0

Pump A (L-7100):

Pump Solvent and Event Table

Time (min)	%ACN	%0.1%	%Wasse	%0	Flow (ml/min)	Event 1	Event 2	Event 3	Event 4
0,0	90,0	0,0	10,0	0,0	0,800				

Autosampler Setup (L-7250):

Syringe Speed: 3	Needle Down Speed: Fast
Syringe Volume: 500 ul	Injection Method: Cut
Lead Volume: 30,00 ul	Rear Volume: 30,00 ul
Needle Wash Strokes: 3	Needle Wash Speed: 5
Injection Port Wash Stroke: 3	Injection Port Wash Speed: 5

Channel 1 Detector (L-7455):

Spectral Bandwidth: AUTO	Spectral Interval: 1600 ms
Absorbance Mode: Normal(2.0AU)	Auto Zero before Injection: YES
Wavelength Range: 210 to 400 nm	Monitoring Wavelength: 220 nm
Start Time: 0,00 min	Stop Time: 30,00 min
Slit: 4 nm	
Check Performance before Series Start: NO	

Method DP for channel 1

Calculation Method:

Calculation Method: AREA%	Peak Quantitation: Area
Peak identification Window: % Time	Concentration data from method.
UNK peaks identification rule: Closest peak	
Update RT in component Table: NO	Do blank subtraction: NO
Do library search: NO	

Component Table

RT (min)	Window (%)	Func1	Func2	Func3	E-Conc	Tolerance (%)
0,01	10,00					