
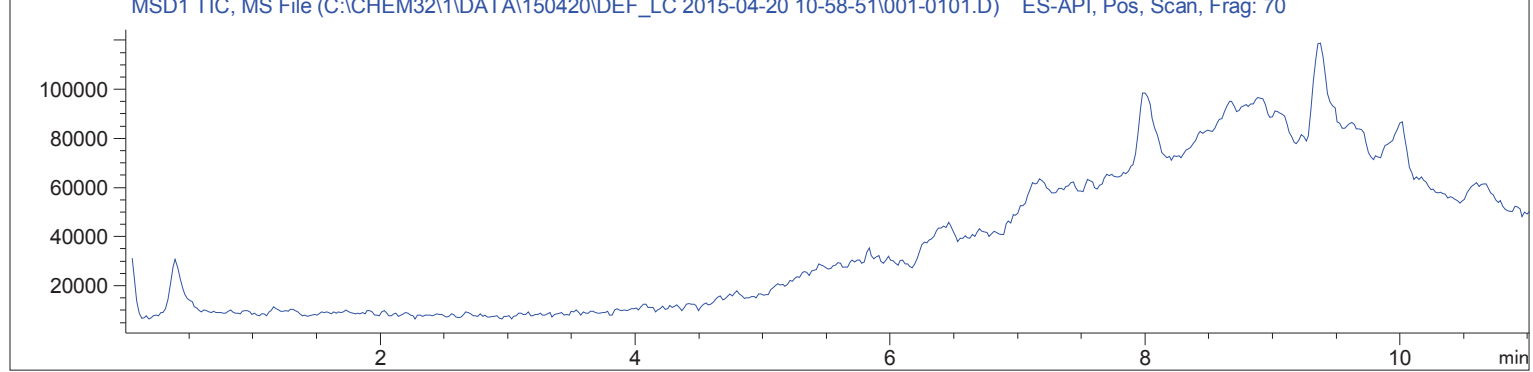
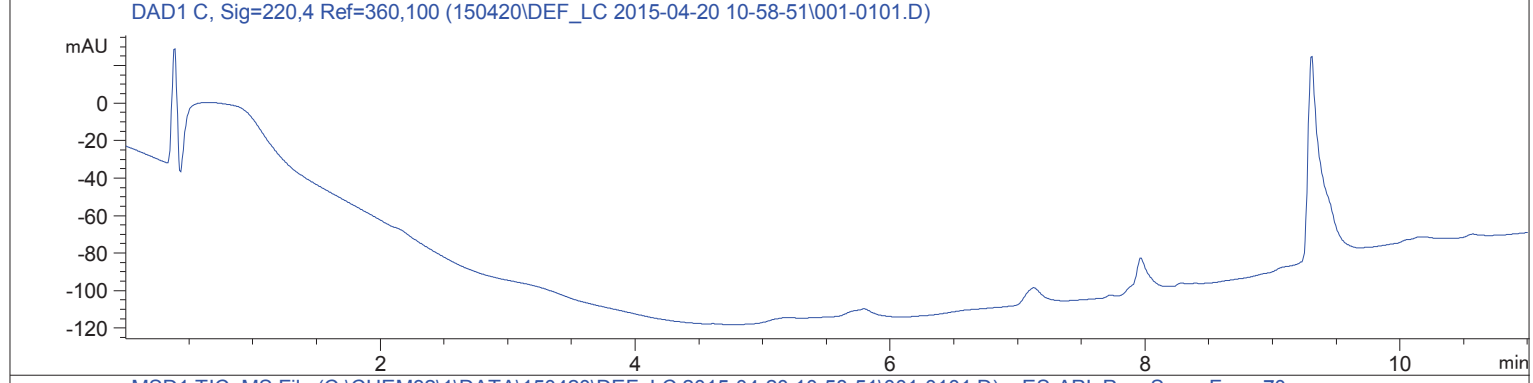


Sample Name: blind

```
=====
Acq. Operator   : SYSTEM                               Seq. Line :    1
Acq. Instrument : LCMS 1                               Location  : Vial 1
Injection Date  : 4/20/2015 11:00:21 AM              Inj       :    1
                                                    Inj Volume: 1.000 µl
Acq. Method     : C:\CHEM32\1\DATA\150420\DEF_LC 2015-04-20 10-58-51\STANDARD_220_254.M
Last changed    : 4/20/2015 10:58:51 AM by SYSTEM
Analysis Method : C:\CHEM32\1\DATA\150420\DEF_LC 2015-04-20 10-58-51\STANDARD_220_254.M (
Sequence Method)
Last changed    : 2/26/2016 10:11:10 AM by SYSTEM
                (modified after loading)
Method Info     : Standard ACN:Wasser 20:80 -> 97:3 Flow 0.4 ml/min 220 nm, 254 nm
=====
```

Additional Info : Peak(s) manually integrated

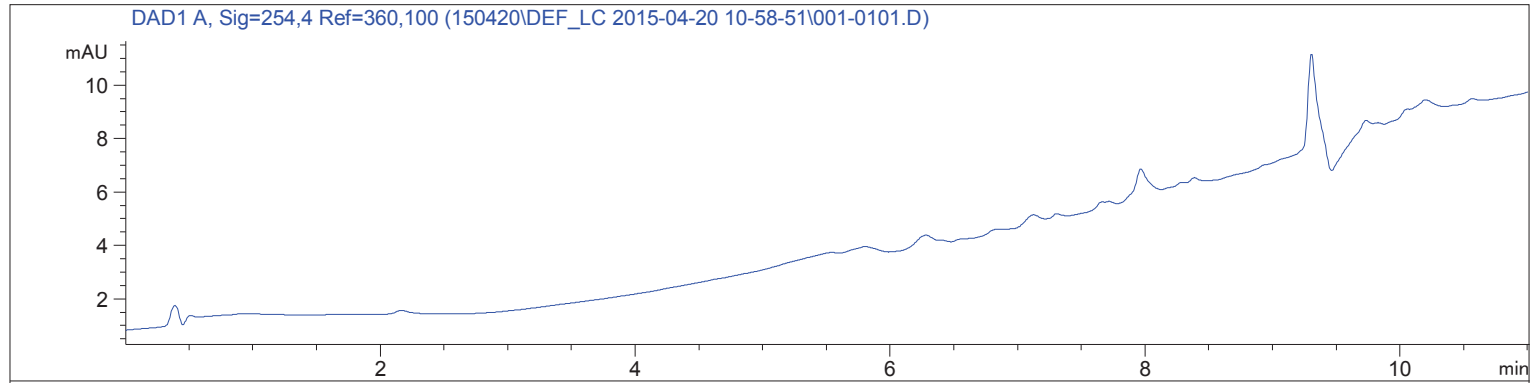

```
=====
                          Area Percent Report
=====
```

```
Sorted By      :      Signal
Multiplier     :      1.0000
Dilution       :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```

No peaks found


=====  
\*\*\* End of Report \*\*\*

Sample Name: blind

=====

Acq. Operator	: SYSTEM	Seq. Line	: 1
Acq. Instrument	: LCMS 1	Location	: Vial 1
Injection Date	: 4/20/2015 11:00:21 AM	Inj	: 1
		Inj Volume	: 1.000 µl
Acq. Method	: C:\CHEM32\1\DATA\150420\DEF_LC 2015-04-20 10-58-51\STANDARD_220_254.M		
Last changed	: 4/20/2015 10:58:51 AM by SYSTEM		
Analysis Method	: C:\CHEM32\1\DATA\150420\DEF_LC 2015-04-20 10-58-51\STANDARD_220_254.M ( Sequence Method)		
Last changed	: 2/26/2016 10:11:28 AM by SYSTEM (modified after loading)		
Method Info	: Standard ACN:Wasser 20:80 -> 97:3 Flow 0.4 ml/min 220 nm, 254 nm		

Additional Info : Peak(s) manually integrated

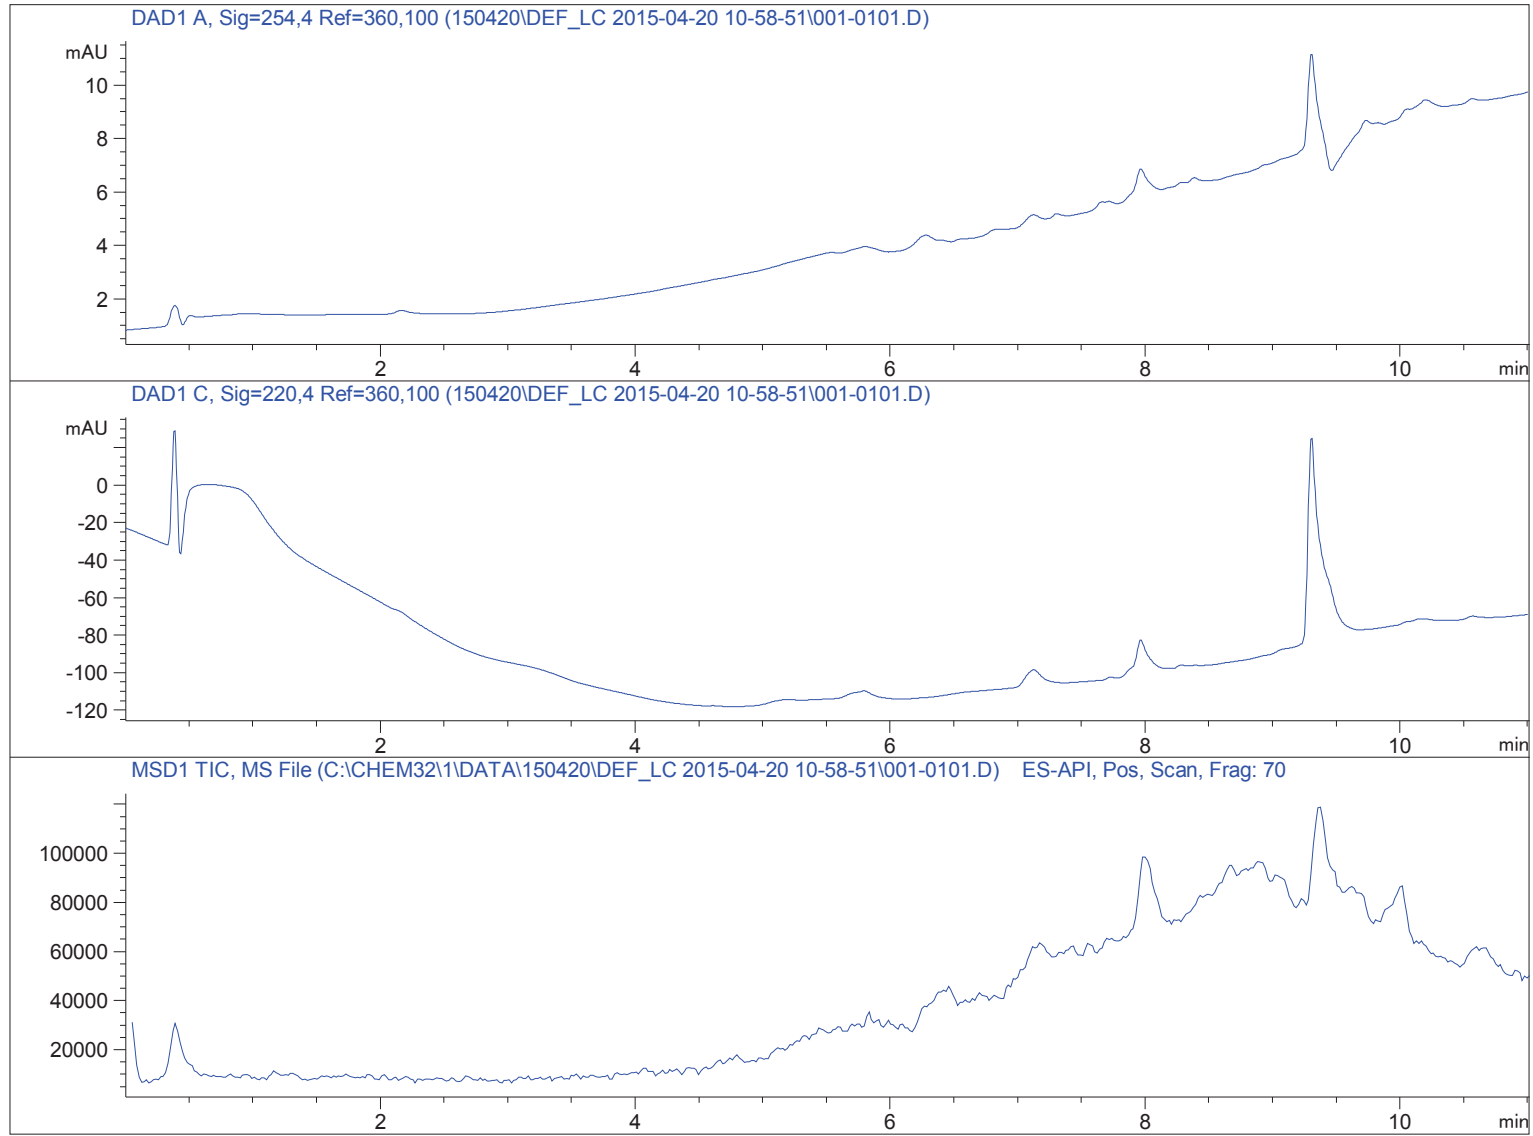

Spectra averaged over upper half of peaks.  
Number of ions per peak: 6  
Display Time Range(+/- mins): 1.0

\*\*\* End of Report \*\*\*