


Sample Name: Test-Phthalat_211124

```

=====
Acq. Operator   : SYSTEM                               Seq. Line :    2
Acq. Instrument : LCMS 1                               Location  : Vial 2
Injection Date  : 11/24/2021 2:30:32 PM              Inj       :    1
                                                    Inj Volume: 1.000 µl

Acq. Method     : C:\CHEM32\1\DATA\211124\211111 2021-11-24 14-13-33\STANDARD_220_254_N2_10.M
Last changed    : 11/24/2021 2:13:33 PM by SYSTEM
Analysis Method : C:\CHEM32\1\DATA\211124\211111 2021-11-24 14-13-33\STANDARD_220_254_N2_10.M
                (Sequence Method)
Last changed    : 11/25/2021 8:41:20 AM by SYSTEM
                (modified after loading)
Method Info     : Standard ACN:Wasser 20:80 -> 97:3 Flow 0.4 ml/min 220 nm, 254 nm
=====

```

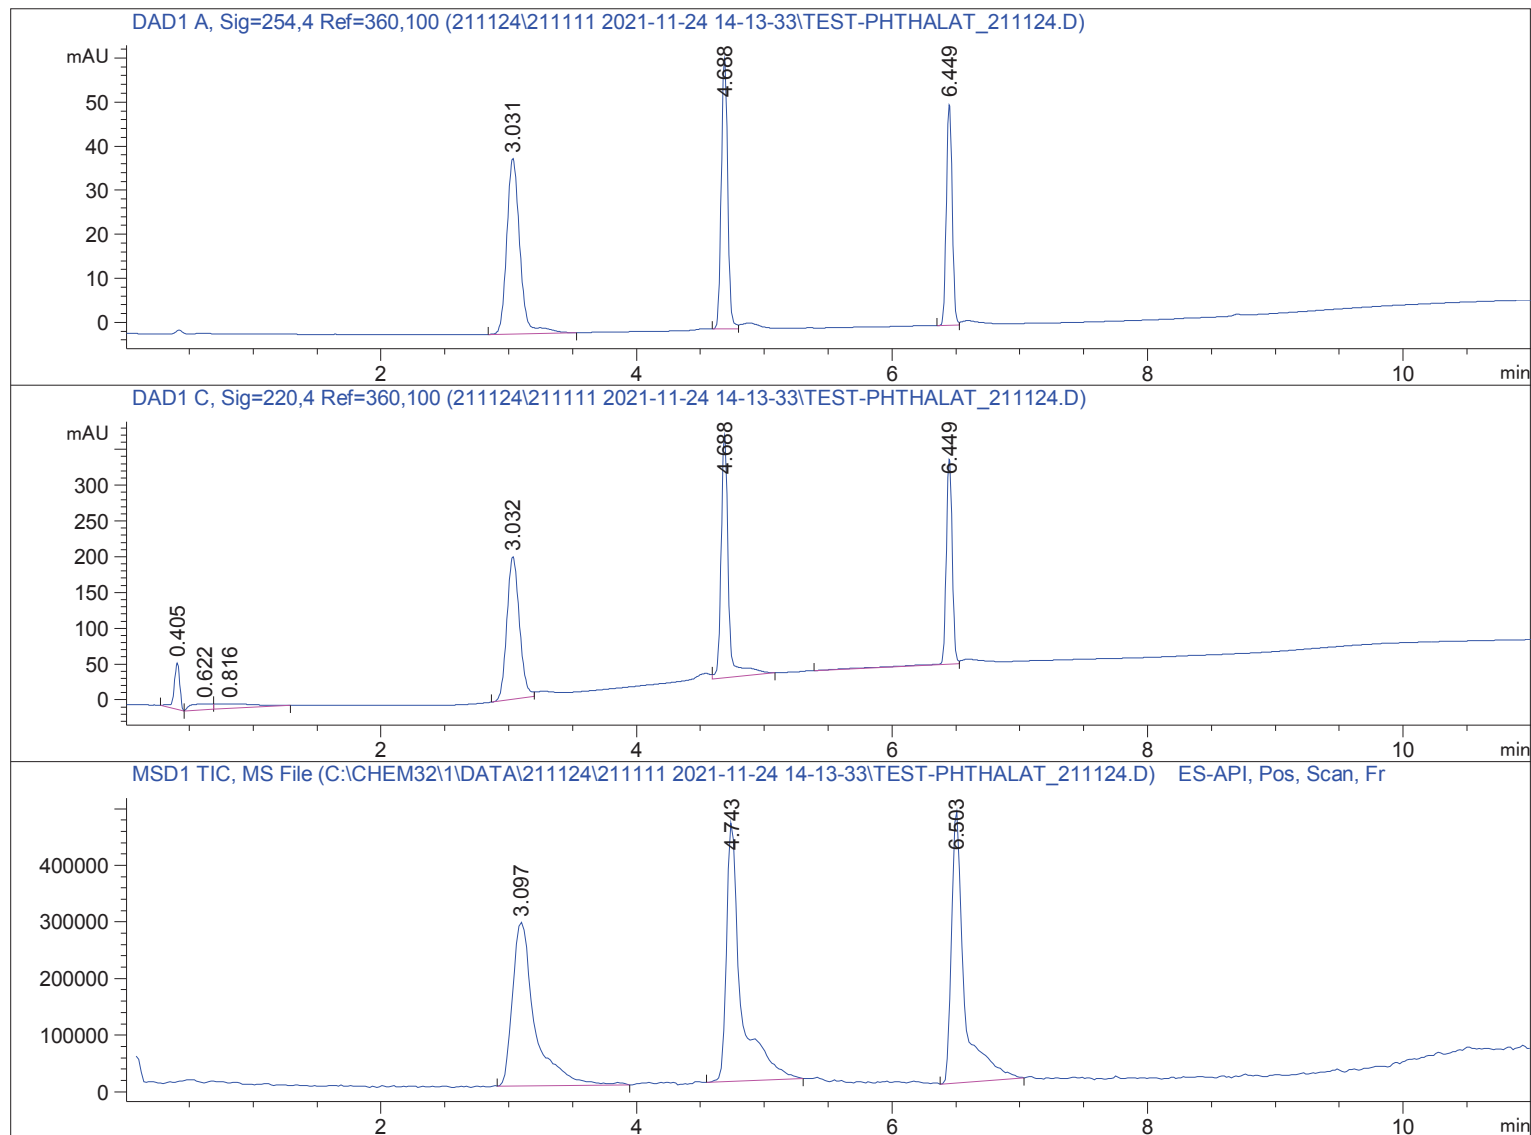

```

=====
                          Area Percent Report
=====

```

```

Sorted By      :      Signal
Multiplier     :      1.0000
Dilution       :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

```

Signal 1: DAD1 A, Sig=254,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	3.031	BB	0.1092	283.70306	39.78479	42.9711
2	4.688	BV	0.0550	216.54660	61.59158	32.7993
3	6.449	BV	0.0490	159.96809	50.49126	24.2296

Totals : 660.21776 151.86763

Signal 2: DAD1 C, Sig=220,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	0.405	BB	0.0493	194.51535	64.35206	4.7138
2	0.622	BV	0.1934	100.72031	8.30786	2.4408
3	0.816	VB	0.2833	140.63425	6.68769	3.4081
4	3.032	BV	0.1057	1359.23596	199.07388	32.9395
5	4.688	VB	0.0610	1371.12500	340.38129	33.2276
6	6.449	VV	0.0508	960.23431	288.58005	23.2701

Totals : 4126.46519 907.38283

Signal 3: MSD1 TIC, MS File


Peak #	RetTime [min]	Type	Width [min]	Area	Height	Area %
1	3.097	BB	0.1815	3.51297e6	2.88736e5	33.2674
2	4.743	BB	0.1099	3.66006e6	4.59551e5	34.6604
3	6.503	BB	0.1038	3.38676e6	4.86486e5	32.0722

Totals : 1.05598e7 1.23477e6

=====
*** End of Report ***

Sample Name: Test-Phthalat_211124

```
=====
Acq. Operator   : SYSTEM                               Seq. Line :    2
Acq. Instrument : LCMS 1                               Location  : Vial 2
Injection Date  : 11/24/2021 2:30:32 PM                Inj       :    1
                                                    Inj Volume: 1.000 µl
Acq. Method     : C:\CHEM32\1\DATA\211124\211111 2021-11-24 14-13-33\STANDARD_220_254_N2_10.M
Last changed    : 11/24/2021 2:13:33 PM by SYSTEM
Analysis Method : C:\CHEM32\1\DATA\211124\211111 2021-11-24 14-13-33\STANDARD_220_254_N2_10.M
                  (Sequence Method)
Last changed    : 11/25/2021 8:41:46 AM by SYSTEM
                  (modified after loading)
Method Info     : Standard ACN:Wasser 20:80 -> 97:3 Flow 0.4 ml/min 220 nm, 254 nm
=====
```

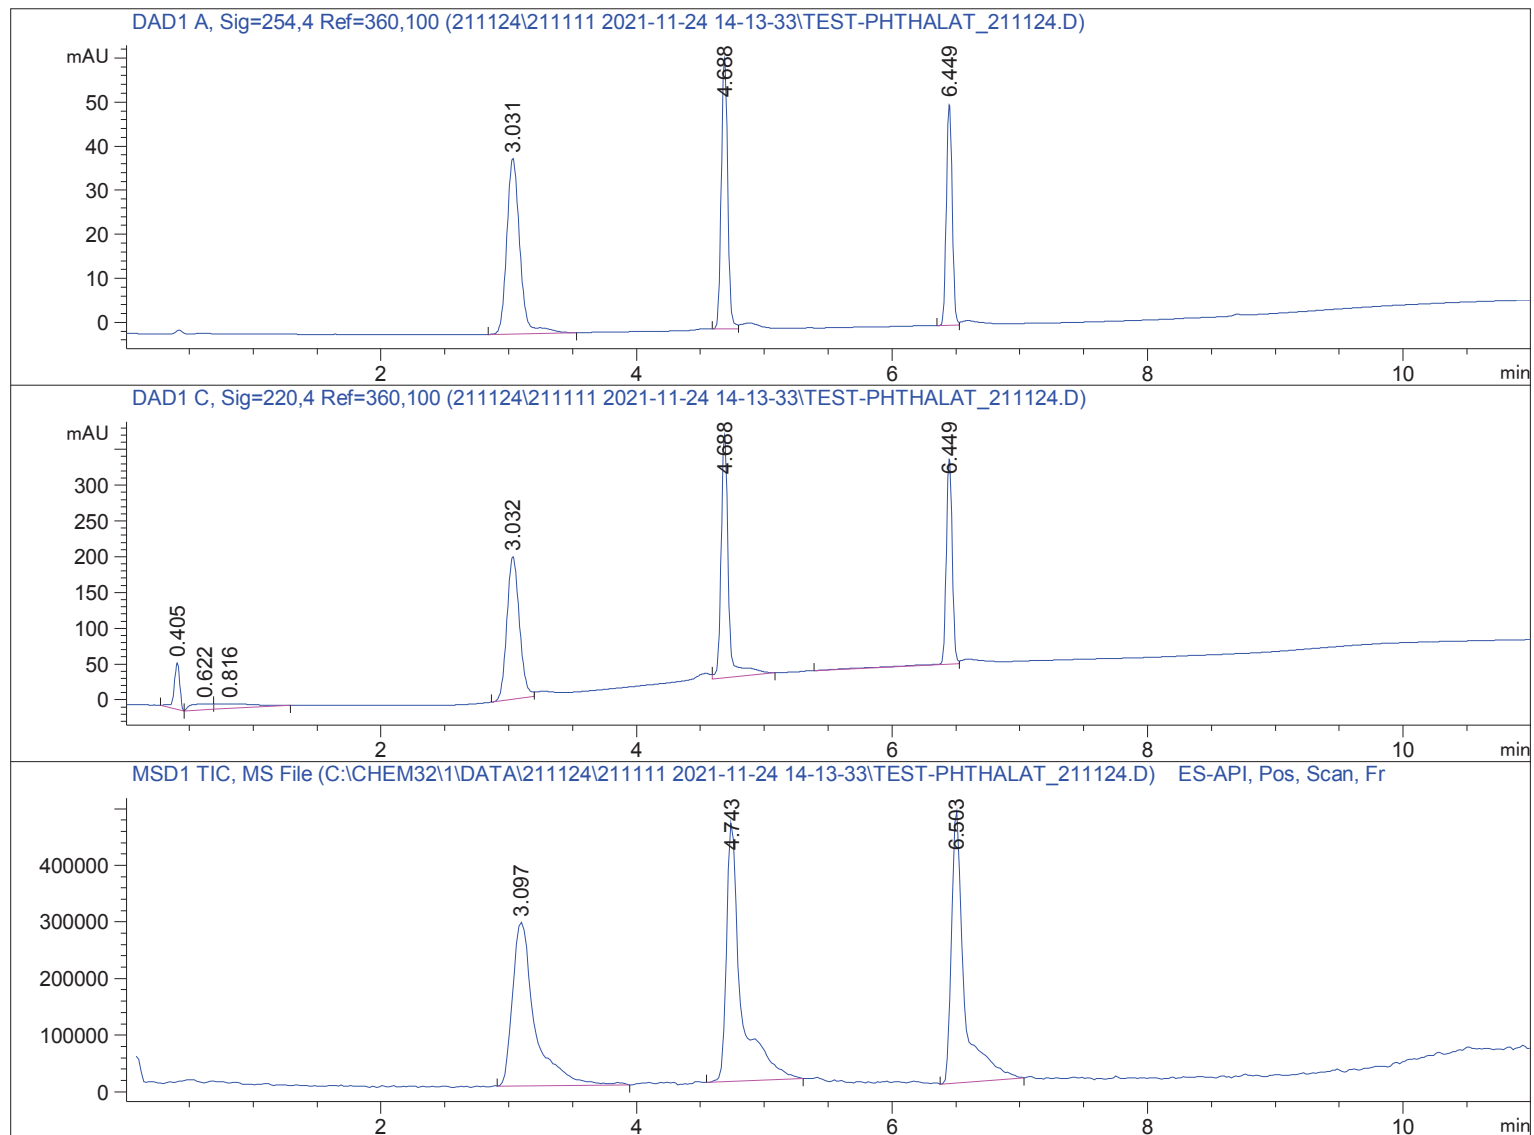

Spectra averaged over upper half of peaks.

Number of ions per peak: 6

Display Time Range(+/- mins): 1.0

Sample Name: Test-Phthalat_211124

DataPath : C:\CHEM32\1\DATA\211124\211111 2021-11-24 14-13-33\TEST-PHTHALAT_211124.D








DateTime: 24 Nov 21 2:30 pm +0100

Operator : SYSTEM

Vial : 2

Sample : Test-Phthalat_211124

Retention : 3.097 minutes

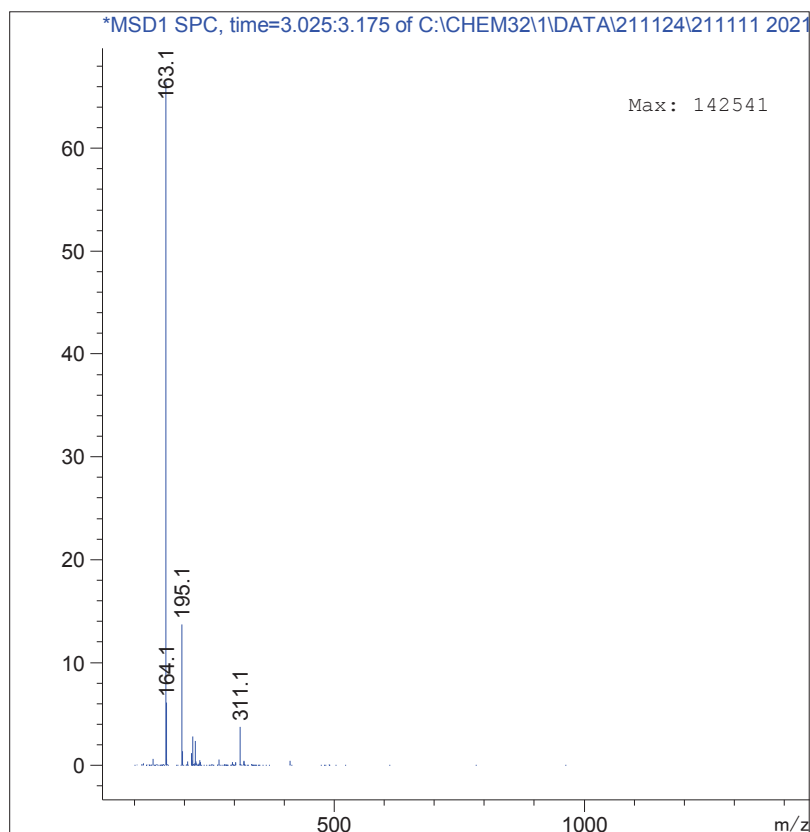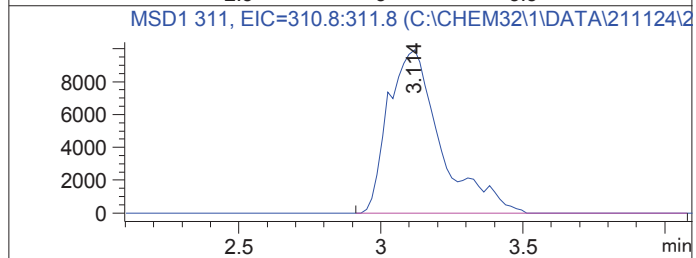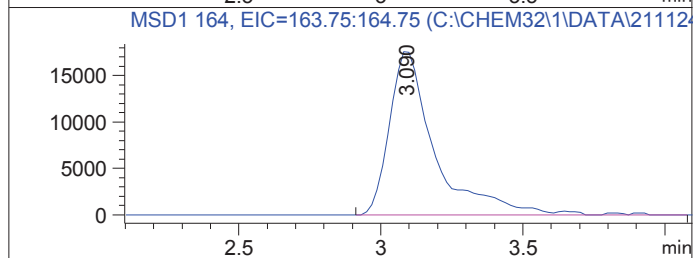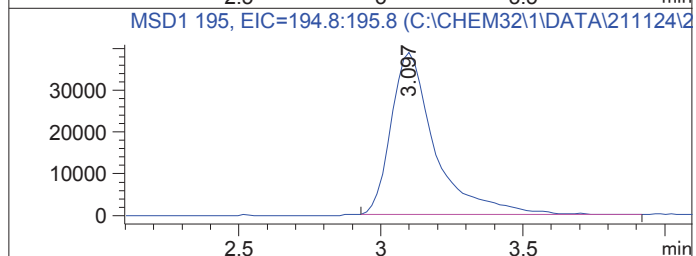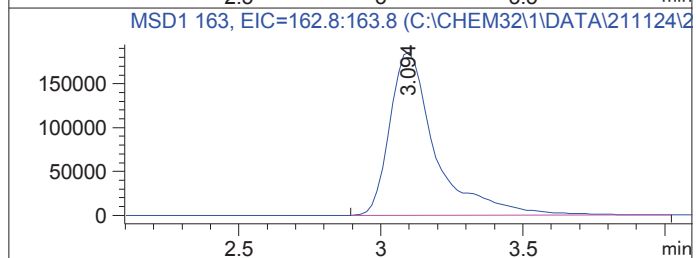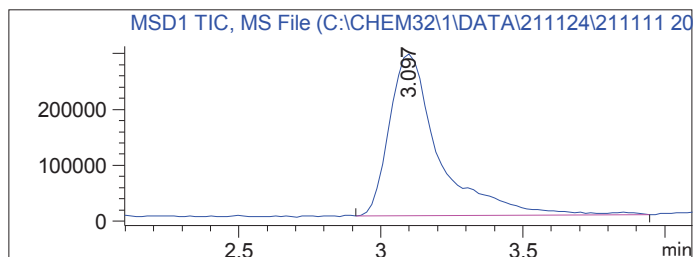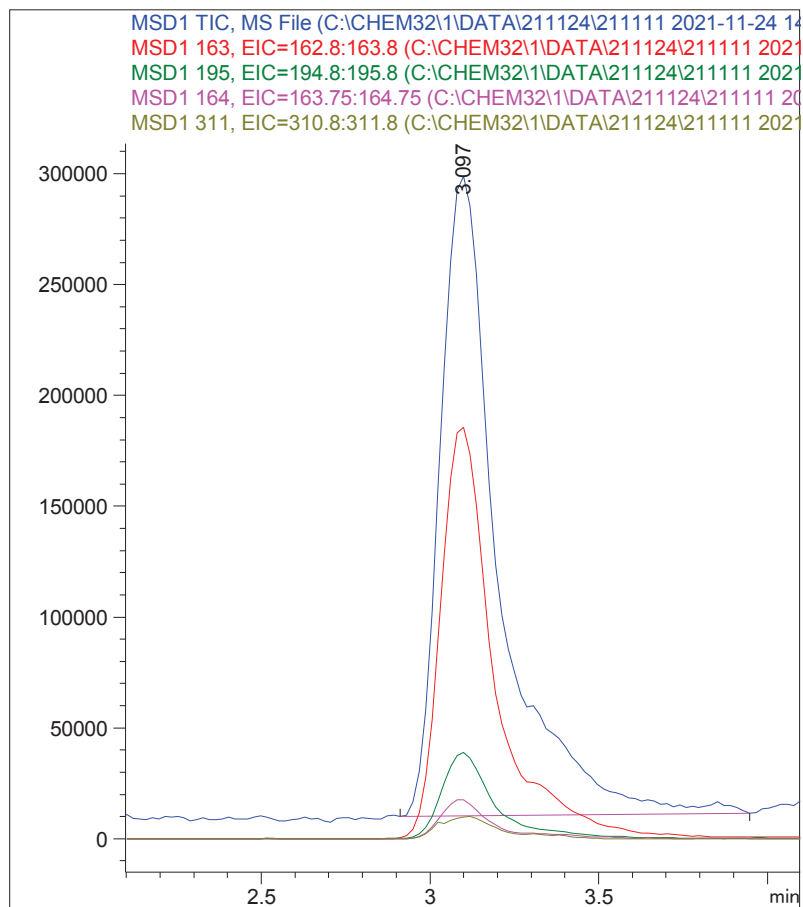

Sample Name: Test-Phthalat_211124

DataPath : C:\CHEM32\1\DATA\211124\211111 2021-11-24 14-13-33\TEST-PHTHALAT_211124.D








DateTime: 24 Nov 21 2:30 pm +0100

Operator : SYSTEM

Vial : 2

Sample : Test-Phthalat_211124

Retention : 4.743 minutes

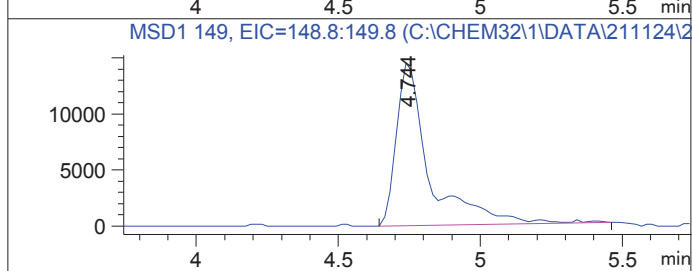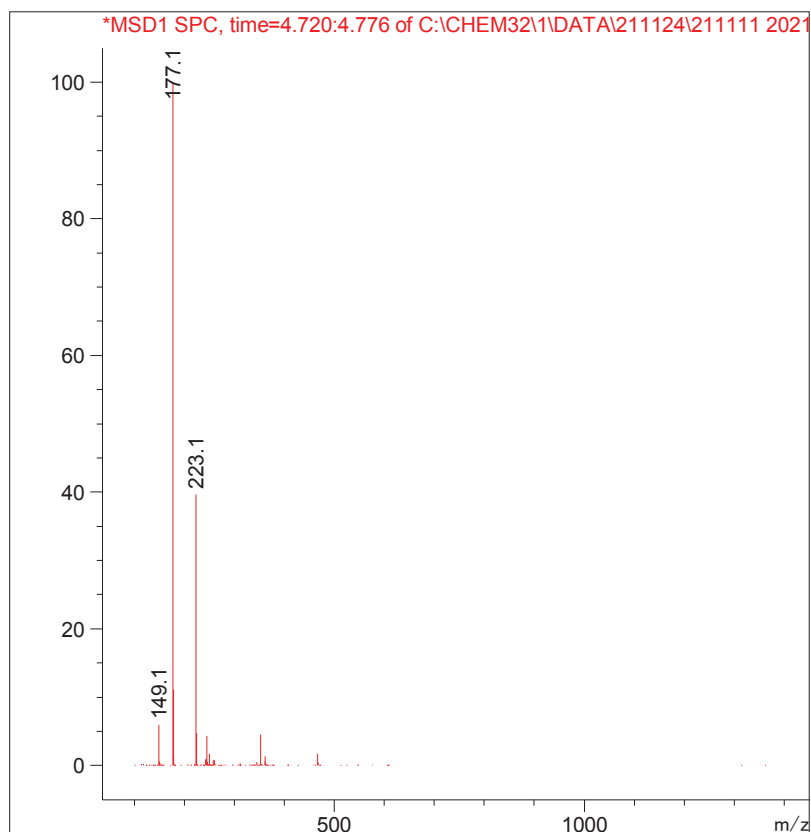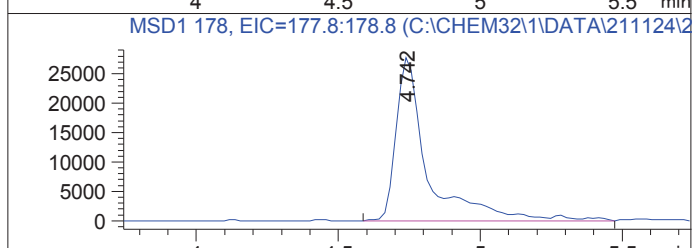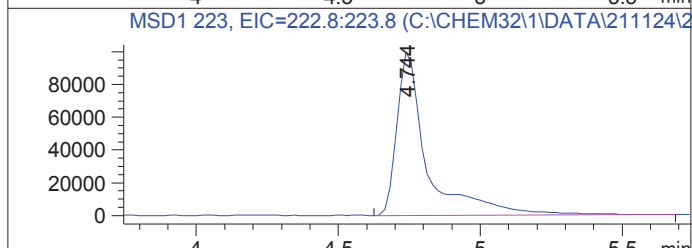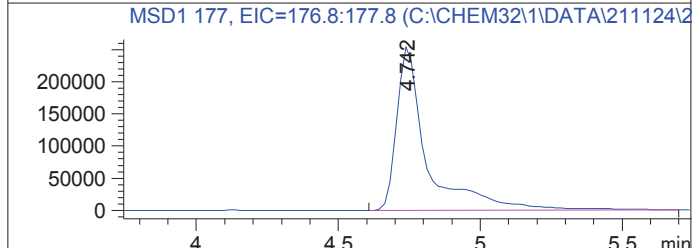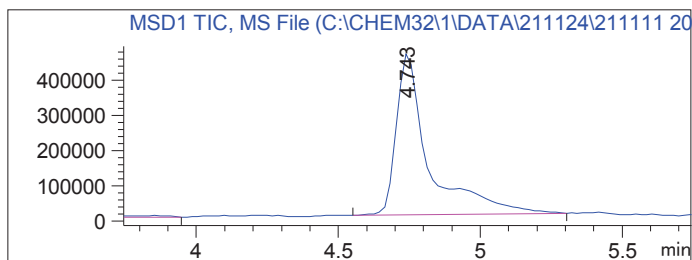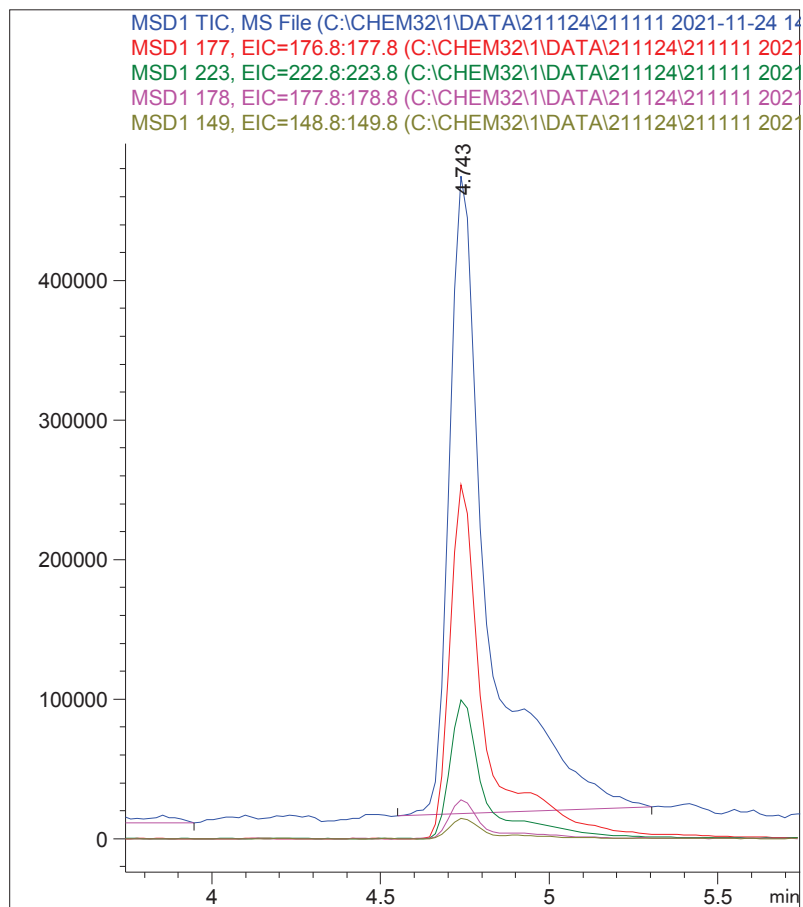

Sample Name: Test-Phthalat_211124

DataPath : C:\CHEM32\1\DATA\211124\211111 2021-11-24 14-13-33\TEST-PHTHALAT_211124.D

DateTime: 24 Nov 21 2:30 pm +0100

Operator : SYSTEM

Vial : 2

Sample : Test-Phthalat_211124

Retention : 6.503 minutes

