


Sample Name: Test160226

=====

Acq. Operator	: SYSTEM	Seq. Line	: 2
Acq. Instrument	: LCMS 1	Location	: Vial 11
Injection Date	: 2/26/2016 11:31:47 AM	Inj	: 1
		Inj Volume	: 1.000 µl
Acq. Method	: C:\CHEM32\1\DATA\160226\DEF_LC 2016-02-26 11-14-45\STANDARD_220_254.M		
Last changed	: 2/26/2016 11:14:45 AM by SYSTEM		
Analysis Method	: C:\CHEM32\1\DATA\160226\DEF_LC 2016-02-26 11-14-45\STANDARD_220_254.M (Sequence Method)		
Last changed	: 2/26/2016 12:26:35 PM by SYSTEM (modified after loading)		
Method Info	: Standard ACN:Wasser 20:80 -> 97:3 Flow 0.4 ml/min 220 nm, 254 nm		

Additional Info : Peak(s) manually integrated

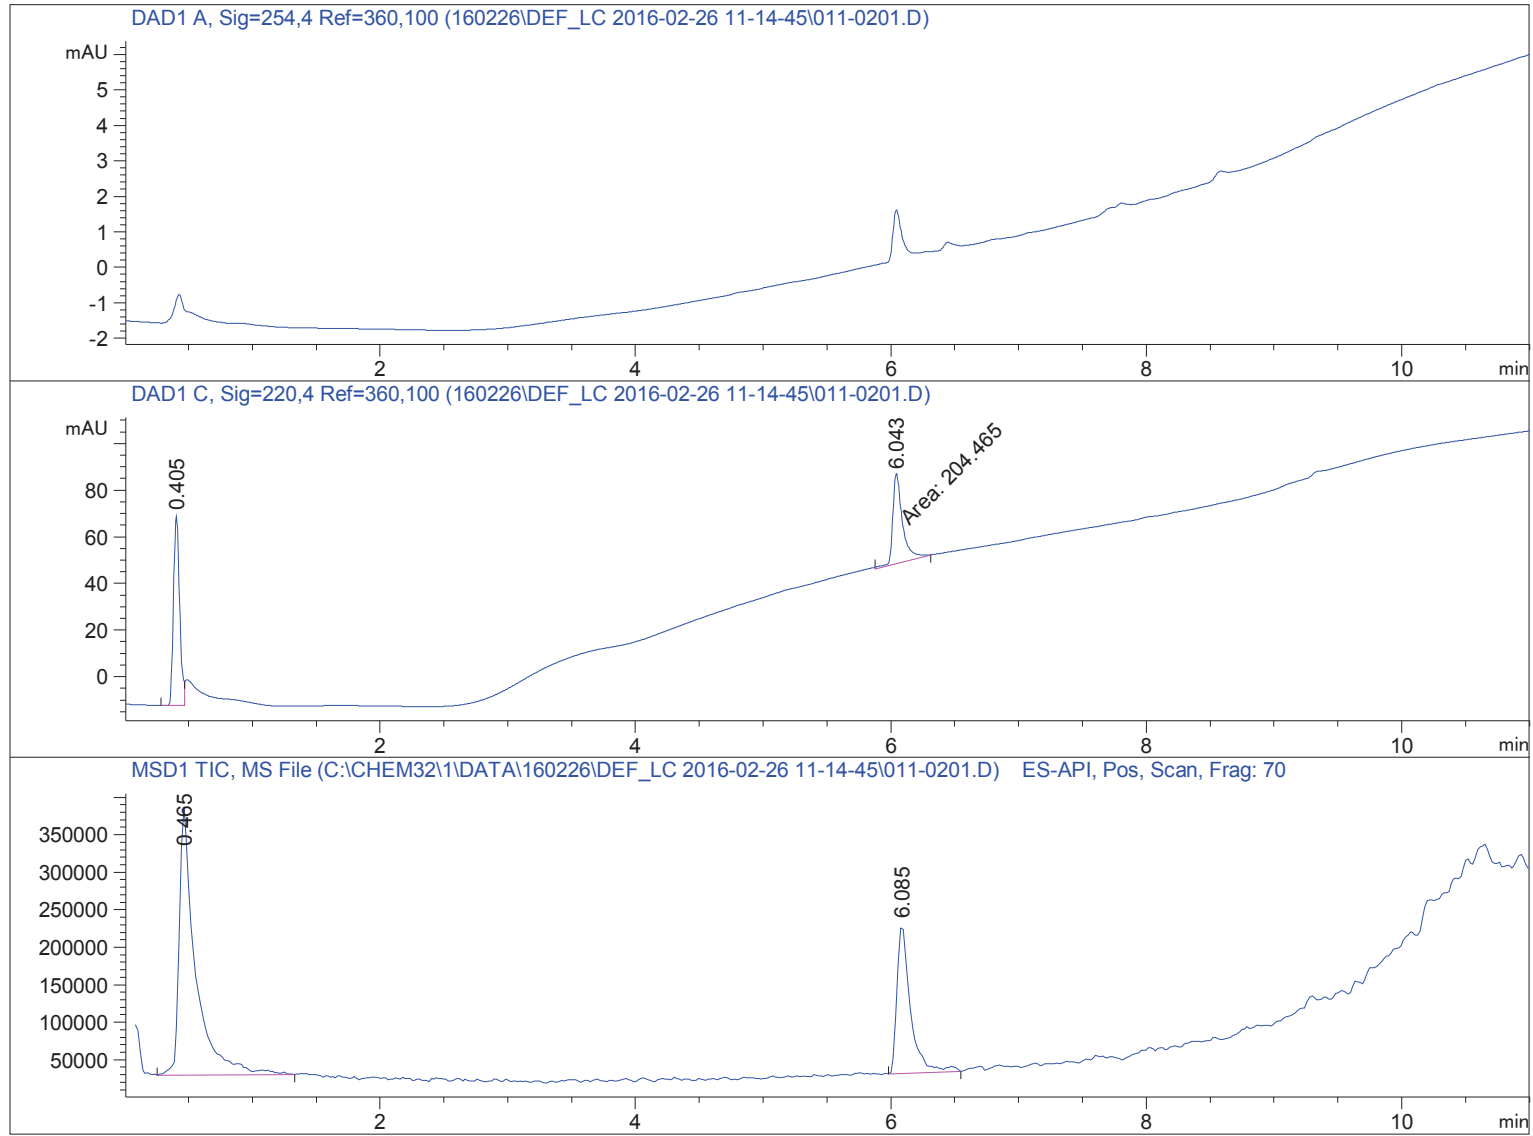

=====
Area Percent Report
=====

Sorted By	:	Signal
Multiplier	:	1.0000
Dilution	:	1.0000

Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=254,4 Ref=360,100

Signal 2: DAD1 C, Sig=220,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	0.405	BV	0.0512	273.33597	81.25916	57.2070
2	6.043	MM	0.0875	204.46538	38.92961	42.7930

Totals : 477.80135 120.18877

Signal 3: MSD1 TIC, MS File

Peak #	RetTime [min]	Type	Width [min]	Area	Height	Area %
1	0.465	BB	0.1212	3.19860e6	3.57889e5	68.8278
2	6.085	BB	0.1076	1.44865e6	1.98958e5	31.1722

Totals : 4.64726e6 5.56848e5


=====
*** End of Report ***

Sample Name: Test160226

=====

Acq. Operator	: SYSTEM	Seq. Line	: 2
Acq. Instrument	: LCMS 1	Location	: Vial 11
Injection Date	: 2/26/2016 11:31:47 AM	Inj	: 1
		Inj Volume	: 1.000 µl
Acq. Method	: C:\CHEM32\1\DATA\160226\DEF_LC 2016-02-26 11-14-45\STANDARD_220_254.M		
Last changed	: 2/26/2016 11:14:45 AM by SYSTEM		
Analysis Method	: C:\CHEM32\1\DATA\160226\DEF_LC 2016-02-26 11-14-45\STANDARD_220_254.M (Sequence Method)		
Last changed	: 2/26/2016 12:26:54 PM by SYSTEM (modified after loading)		
Method Info	: Standard ACN:Wasser 20:80 -> 97:3 Flow 0.4 ml/min 220 nm, 254 nm		

Additional Info : Peak(s) manually integrated

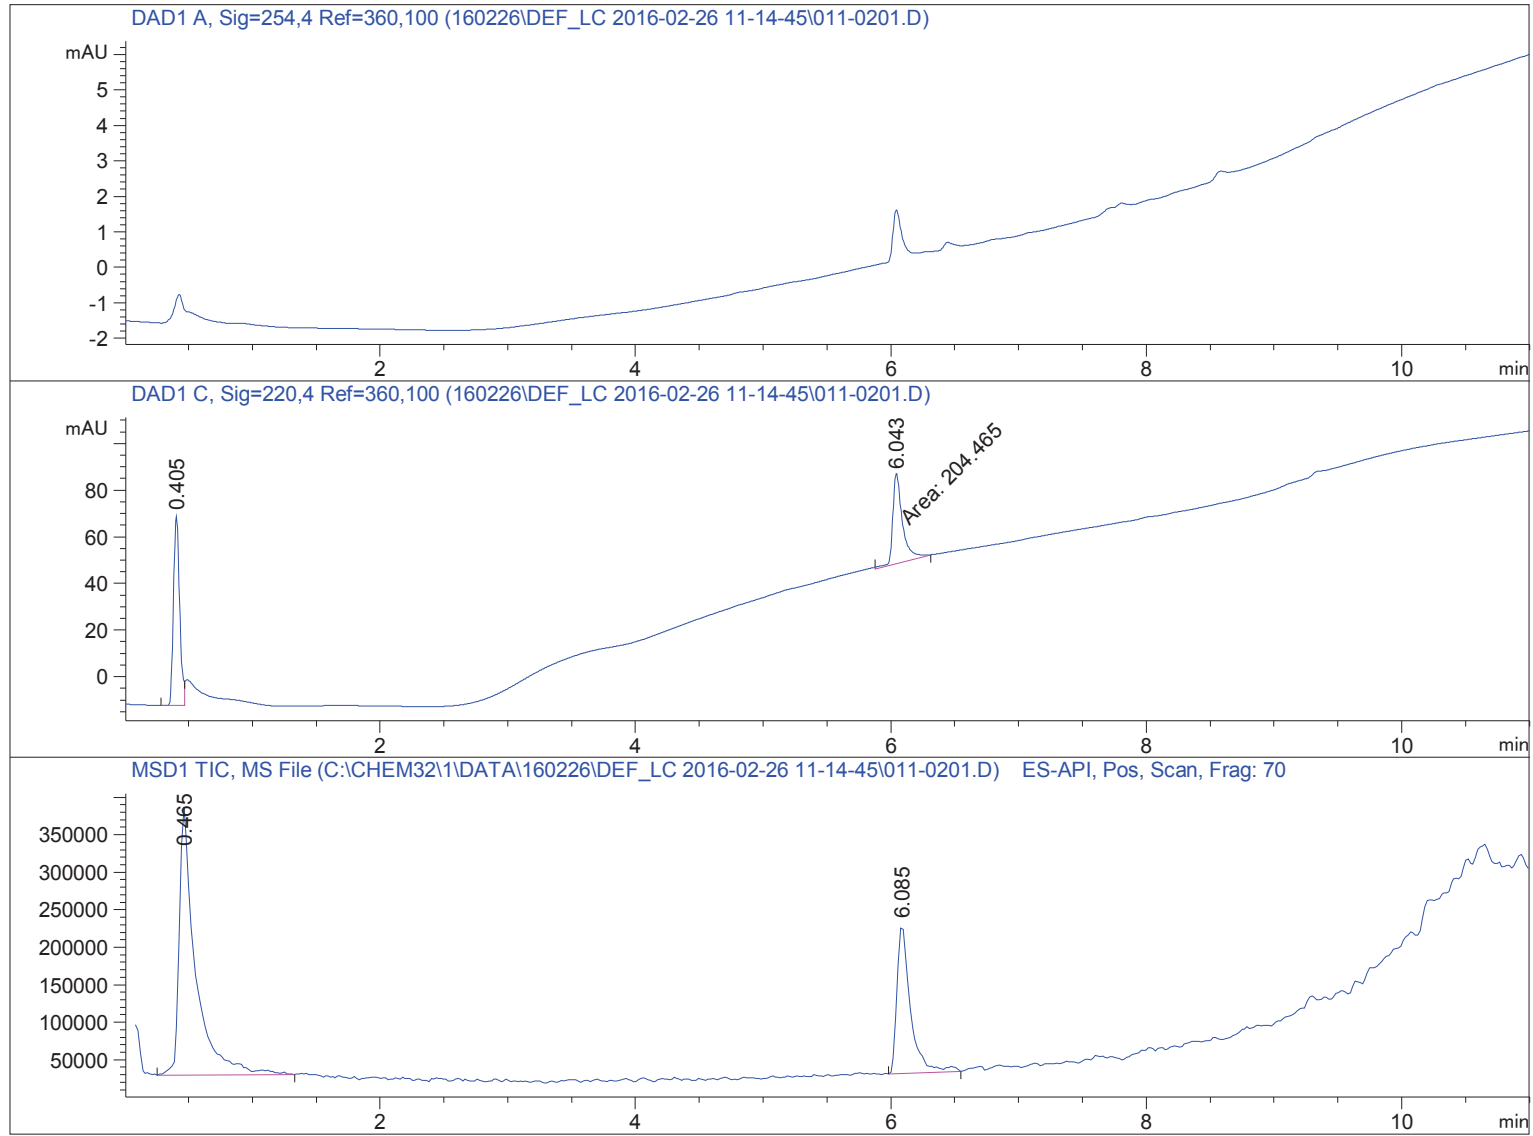

Spectra averaged over upper half of peaks.
Number of ions per peak: 6
Display Time Range(+/- mins): 1.0

Sample Name: Test160226

DataPath : C:\CHEM32\1\DATA\160226\DEF_LC 2016-02-26 11-14-45\011-0201.D






DateTime: 26 Feb 16 11:31 am +0100

Operator : SYSTEM

Vial : 11

Sample : Test160226

Retention : 0.465 minutes

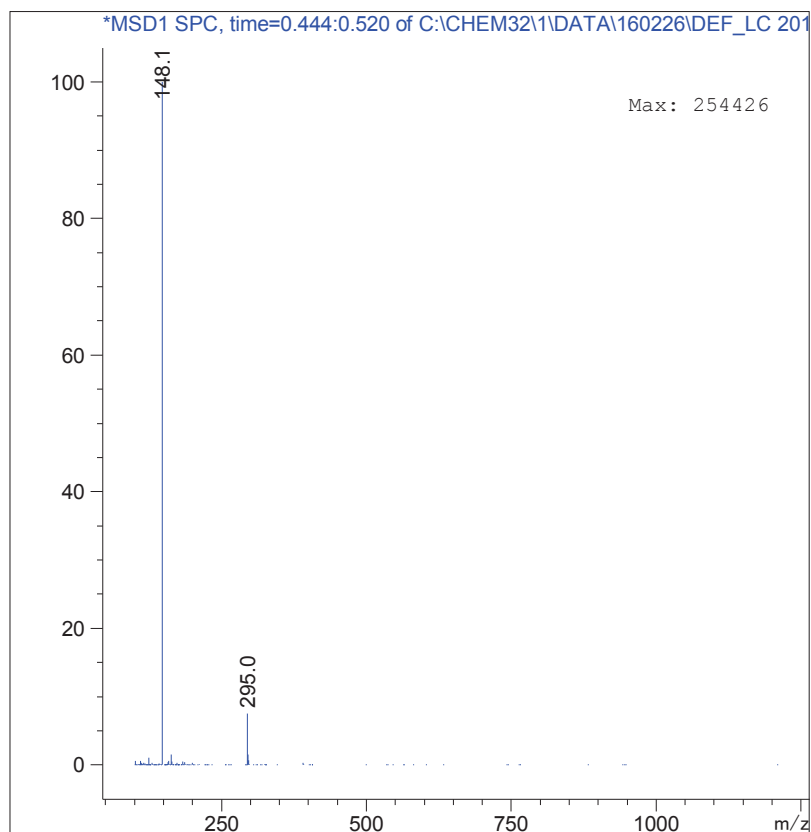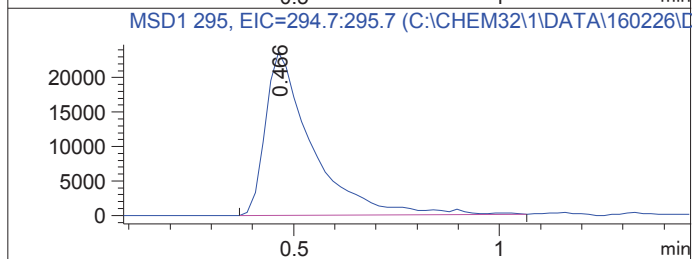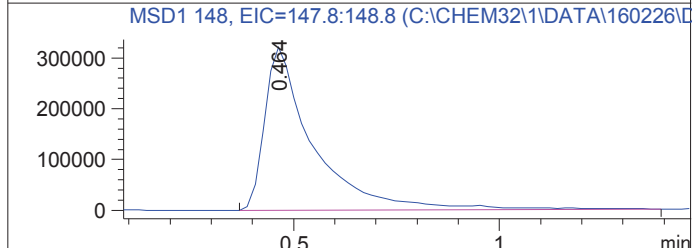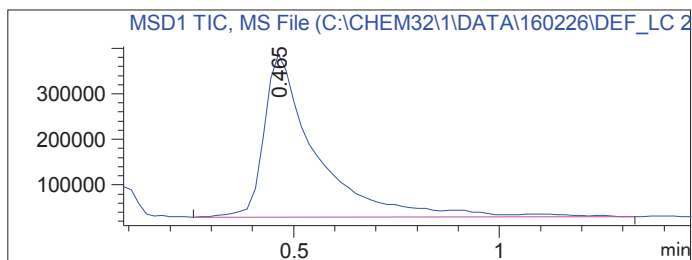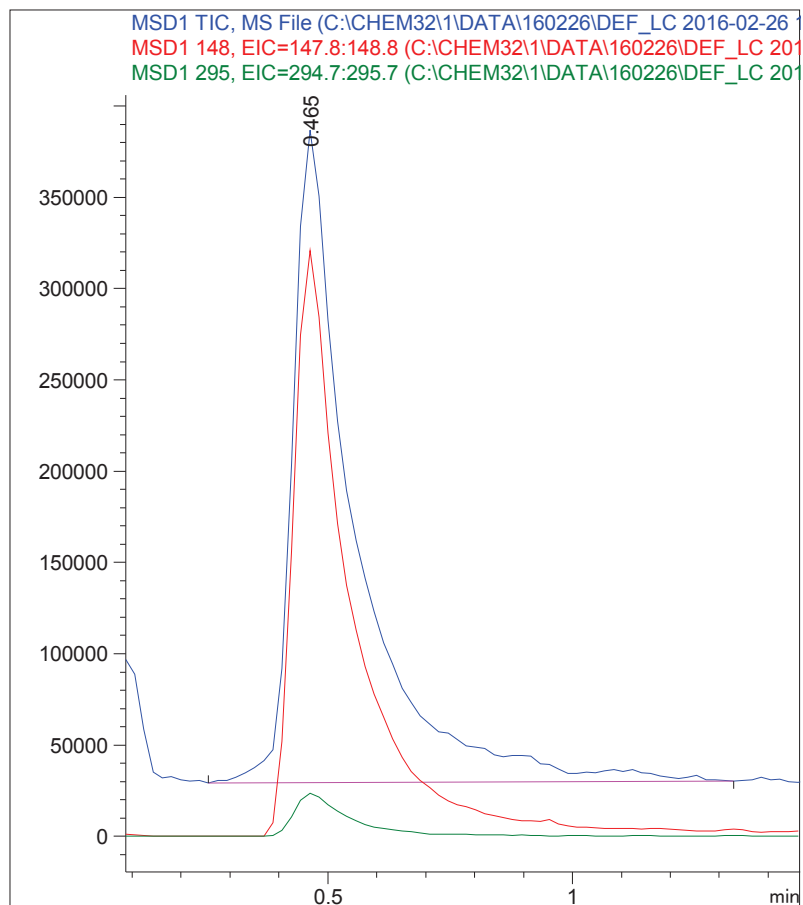

Sample Name: Test160226

DataPath : C:\CHEM32\1\DATA\160226\DEF_LC 2016-02-26 11-14-45\011-0201.D

DateTime: 26 Feb 16 11:31 am +0100

Operator : SYSTEM

Vial : 11

Sample : Test160226

Retention : 6.085 minutes

