
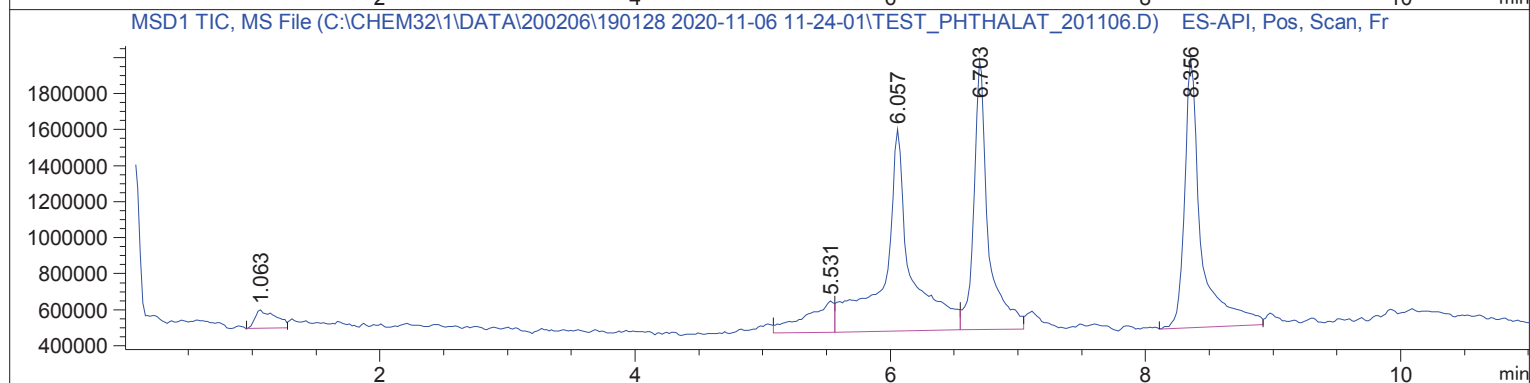
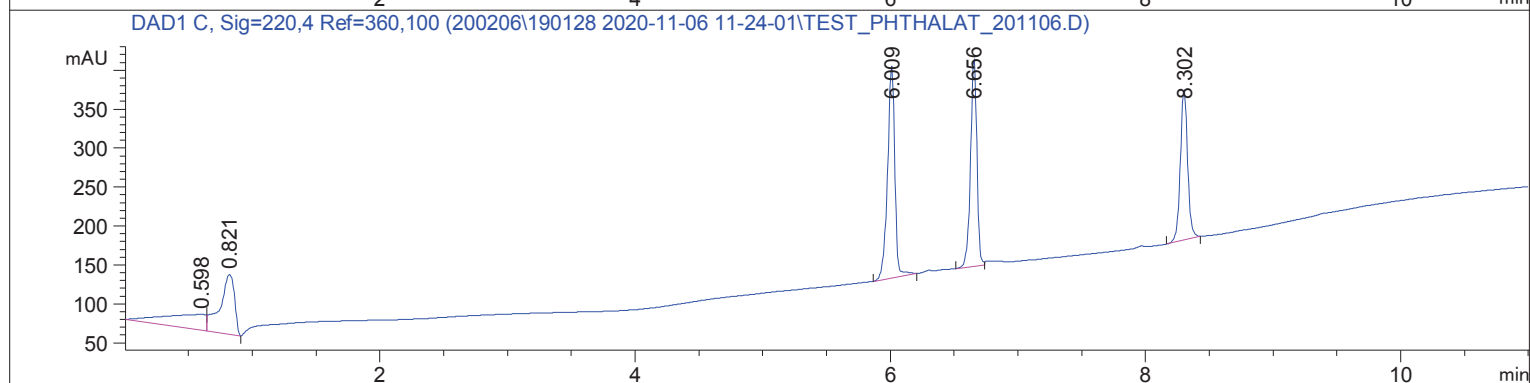


Sample Name: Test_Phthalat_201106

```
=====
Acq. Operator   : SYSTEM                      Seq. Line :    2
Acq. Instrument : LCMS 1                     Location  : Vial 2
Injection Date  : 11/6/2020 11:41:03 AM      Inj       :    1
                                           Inj Volume: 1.000 µl
Acq. Method     : C:\CHEM32\1\DATA\200206\190128 2020-11-06 11-24-01\STANDARD_220_254.M
Last changed    : 11/6/2020 11:24:01 AM by SYSTEM
Analysis Method : C:\CHEM32\1\DATA\200206\190128 2020-11-06 11-24-01\STANDARD_220_254.M (
Sequence Method)
Last changed    : 11/6/2020 12:08:47 PM by SYSTEM
                 (modified after loading)
Method Info     : Standard ACN:Wasser 20:80 -> 97:3 Flow 0.4 ml/min 220 nm, 254 nm
=====
```

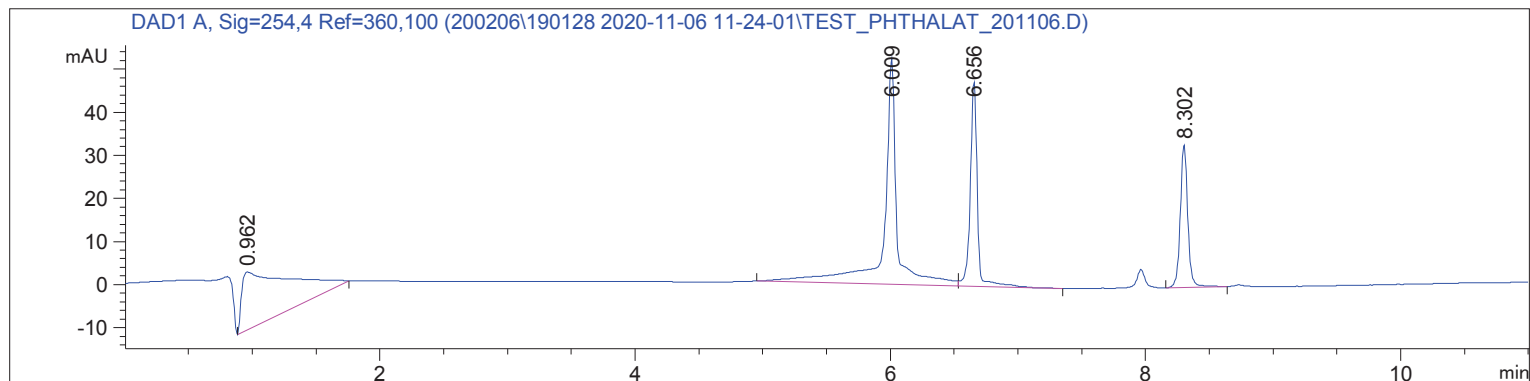

```
=====
                          Area Percent Report
=====
```

```
Sorted By      :      Signal
Multiplier     :      1.0000
Dilution       :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```

Signal 1: DAD1 A, Sig=254,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	0.962	BB	0.3168	336.34299	13.40255	32.6393
2	6.009	BV	0.0975	375.35077	52.46039	36.4246
3	6.656	VB	0.0595	184.84987	47.44392	17.9381
4	8.302	BB	0.0631	133.94205	33.15464	12.9980

Totals : 1030.48567 146.46150

Signal 2: DAD1 C, Sig=220,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	0.598	BV	0.2644	436.21744	20.32707	11.4759
2	0.821	VB	0.1187	609.30762	76.64772	16.0294
3	6.009	BB	0.0601	1076.27380	272.50797	28.3142
4	6.656	BV	0.0543	916.29913	265.03436	24.1057
5	8.302	BB	0.0619	763.07898	193.76144	20.0748

Totals : 3801.17697 828.27856

Signal 3: MSD1 TIC, MS File


Peak #	RetTime [min]	Type	Width [min]	Area	Height	Area %
1	1.063	BV	0.1532	1.16712e6	1.04239e5	2.5839
2	5.531	VV	0.1921	2.67517e6	1.72604e5	5.9226
3	6.057	VV	0.1862	1.62232e7	1.11842e6	35.9171
4	6.703	VV	0.1126	1.16864e7	1.51490e6	25.8729
5	8.356	BV	0.1335	1.34166e7	1.48771e6	29.7035

Totals : 4.51686e7 4.39787e6

=====
*** End of Report ***

Sample Name: Test_Phthalat_201106

```
=====
Acq. Operator   : SYSTEM                      Seq. Line :    2
Acq. Instrument : LCMS 1                     Location  : Vial 2
Injection Date  : 11/6/2020 11:41:03 AM      Inj       :    1
                                           Inj Volume: 1.000 µl
Acq. Method     : C:\CHEM32\1\DATA\200206\190128 2020-11-06 11-24-01\STANDARD_220_254.M
Last changed    : 11/6/2020 11:24:01 AM by SYSTEM
Analysis Method : C:\CHEM32\1\DATA\200206\190128 2020-11-06 11-24-01\STANDARD_220_254.M (
Sequence Method)
Last changed    : 11/6/2020 12:09:09 PM by SYSTEM
                 (modified after loading)
Method Info     : Standard ACN:Wasser 20:80 -> 97:3 Flow 0.4 ml/min 220 nm, 254 nm
=====
```

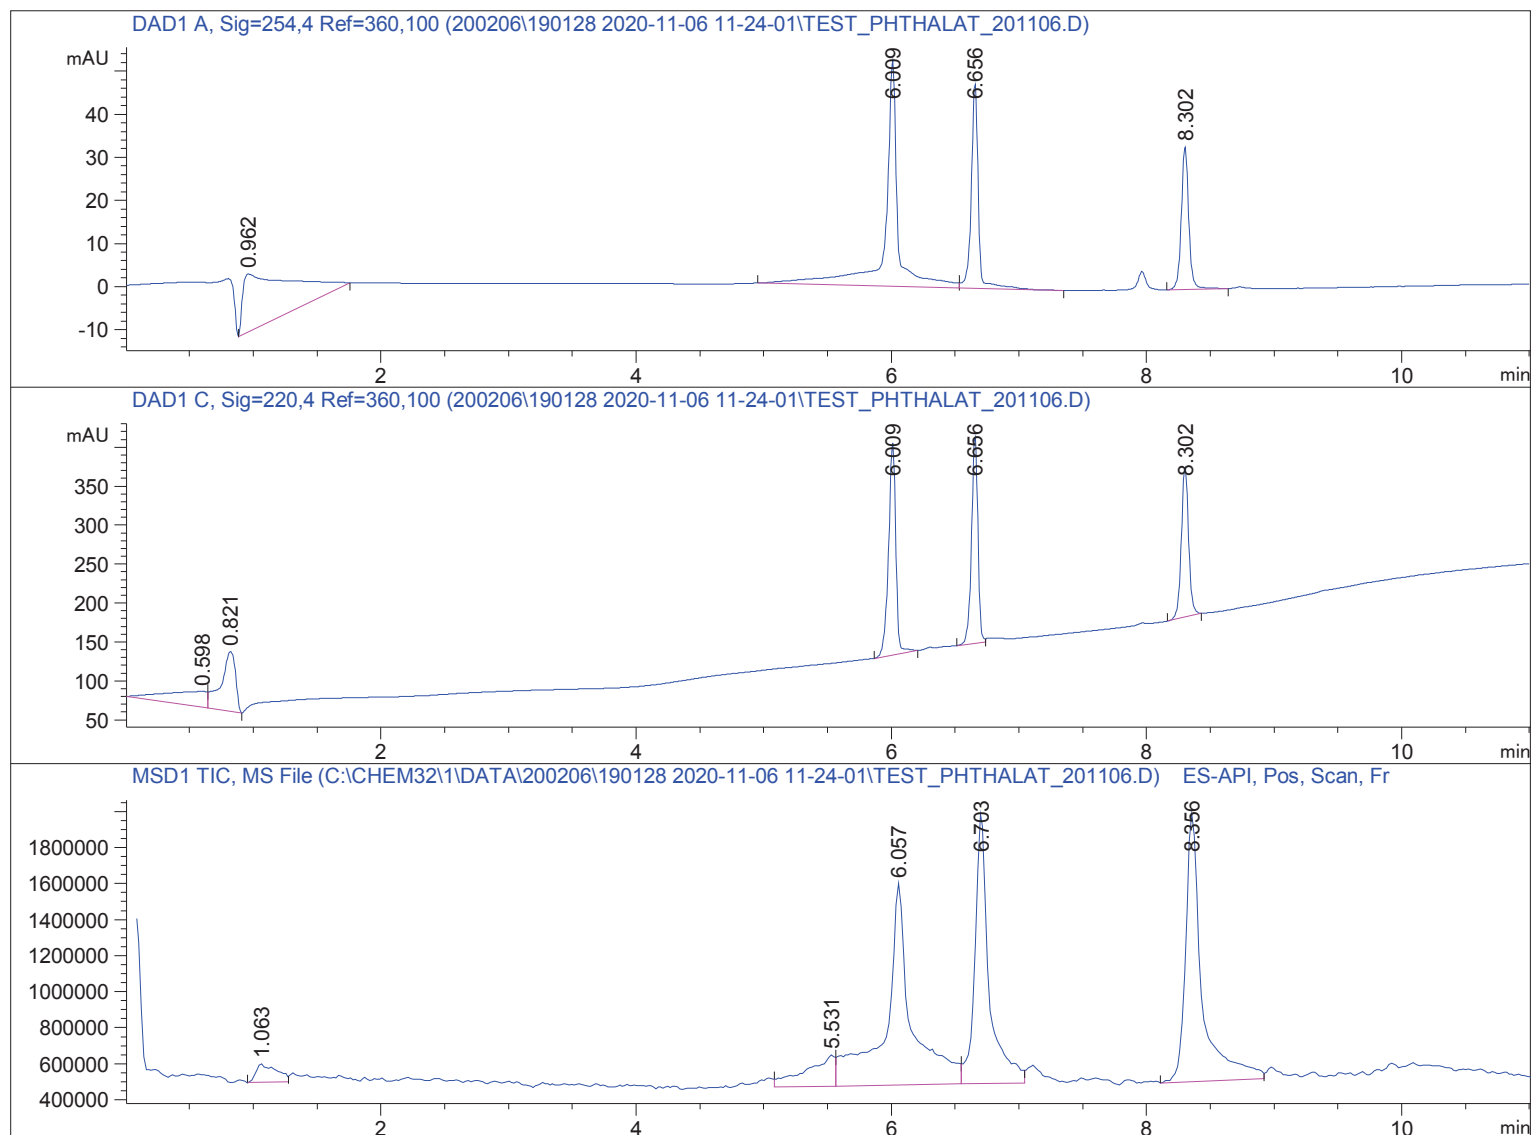

Spectra averaged over upper half of peaks.

Number of ions per peak: 6

Display Time Range(+/- mins): 1.0

Sample Name: Test_Phthalat_201106

DataPath : C:\CHEM32\1\DATA\200206\190128 2020-11-06 11-24-01\TEST_PHTHALAT_201106.D









DateTime : 11/06/2020 00:09:13 pm

Operator : SYSTEM

Vial : 2

Sample : Test_Phthalat_201106

Retention : 1.063 minutes

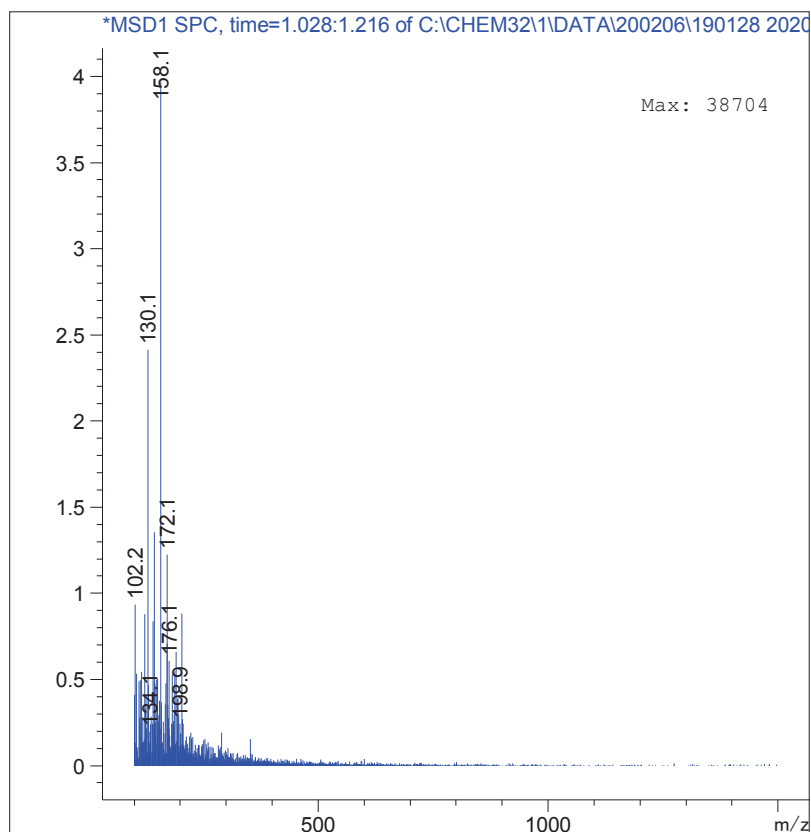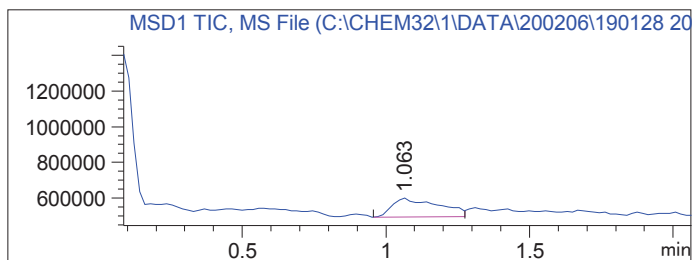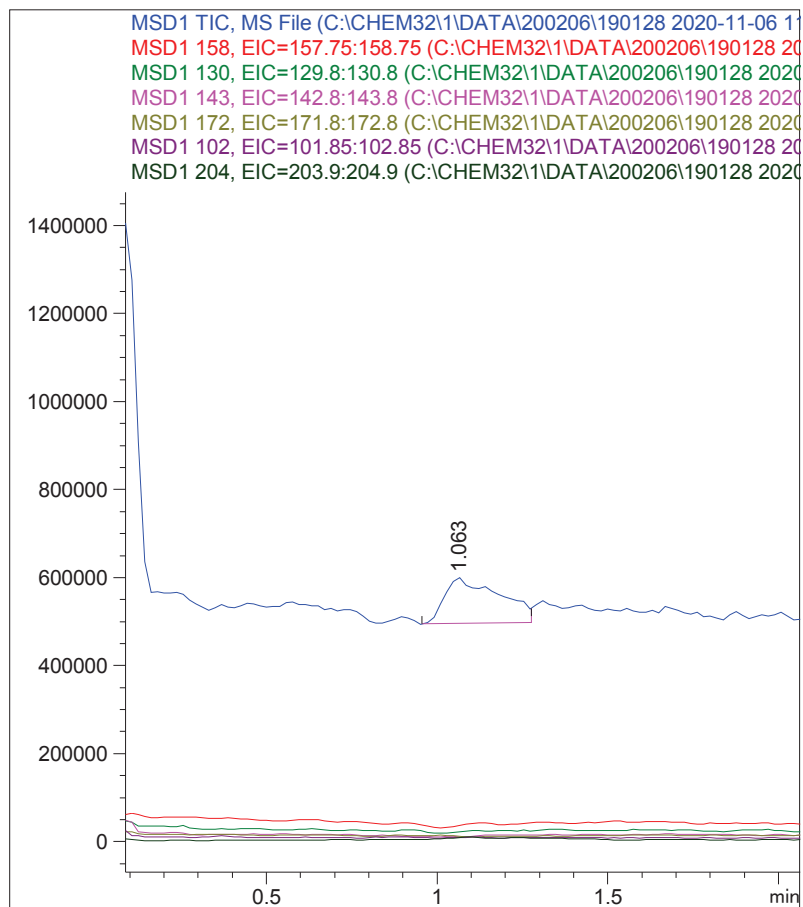

Sample Name: Test_Phthalat_201106

DataPath : C:\CHEM32\1\DATA\200206\190128 2020-11-06 11-24-01\TEST_PHTHALAT_201106.D










DateTime : 11/06/2020 00:09:13 pm

Operator : SYSTEM

Vial : 2

Sample : Test_Phthalat_201106

Retention : 5.531 minutes

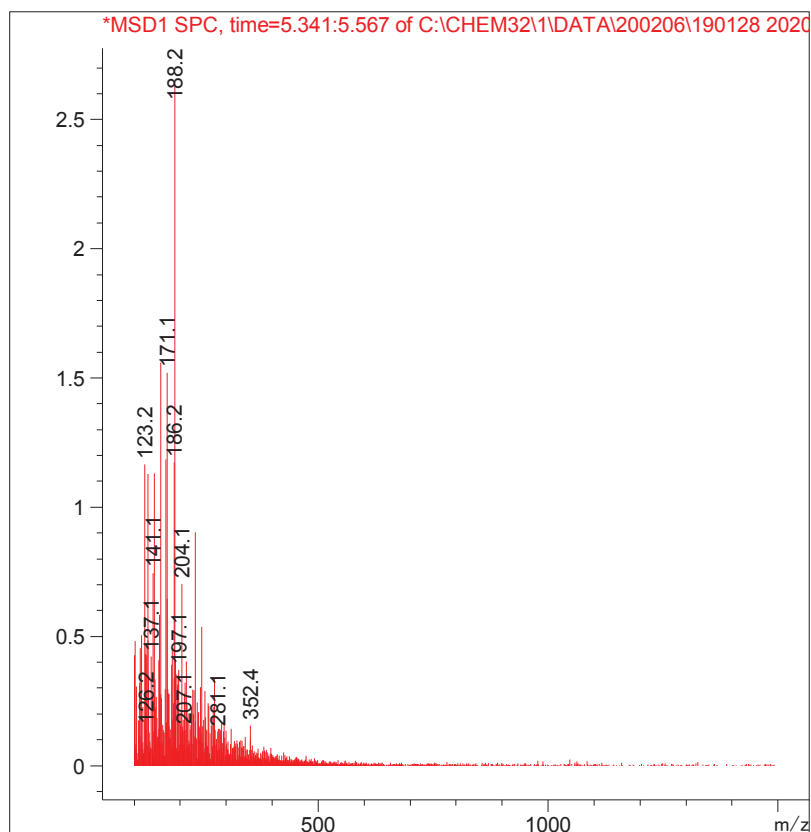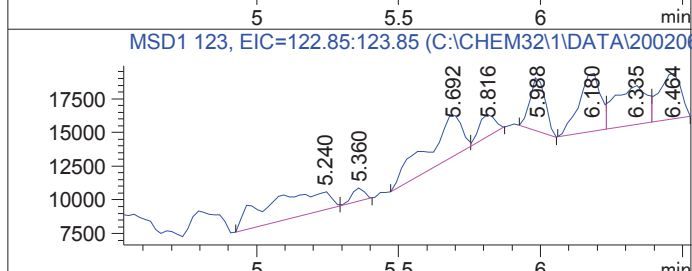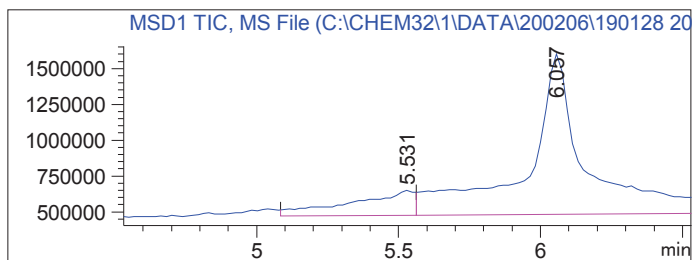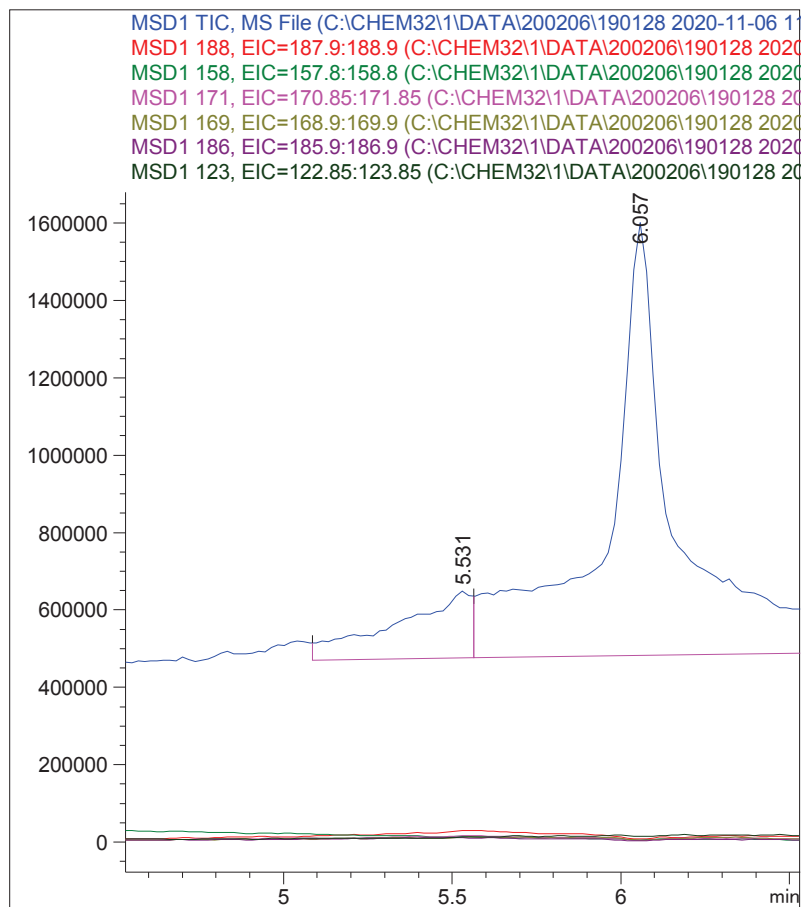

Sample Name: Test_Phthalat_201106

DataPath : C:\CHEM32\1\DATA\200206\190128 2020-11-06 11-24-01\TEST_PHTHALAT_201106.D








DateTime : 11/06/2020 00:09:13 pm

Operator : SYSTEM

Vial : 2

Sample : Test_Phthalat_201106

Retention : 6.057 minutes

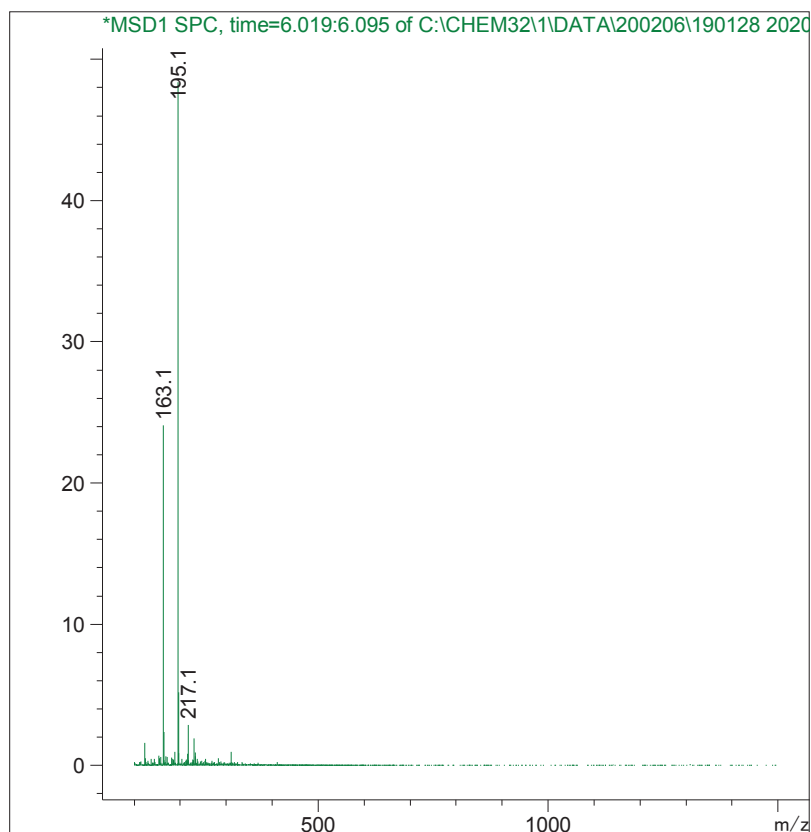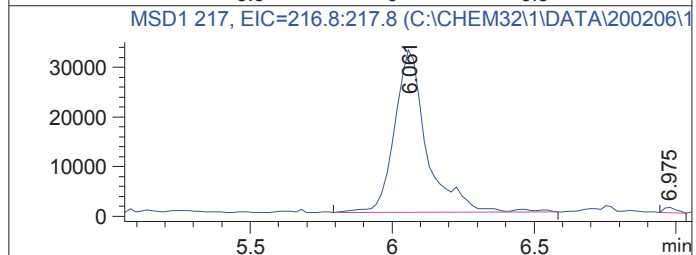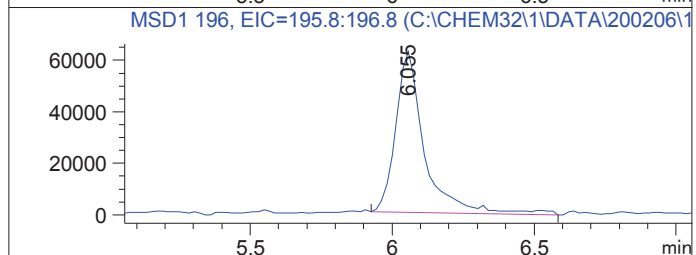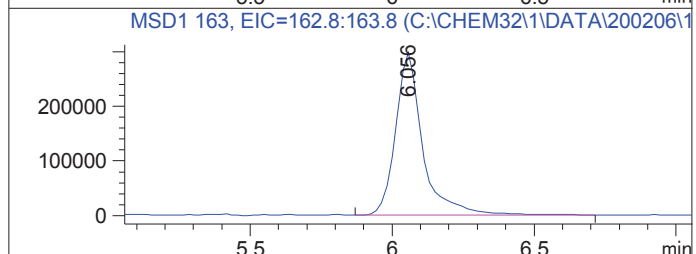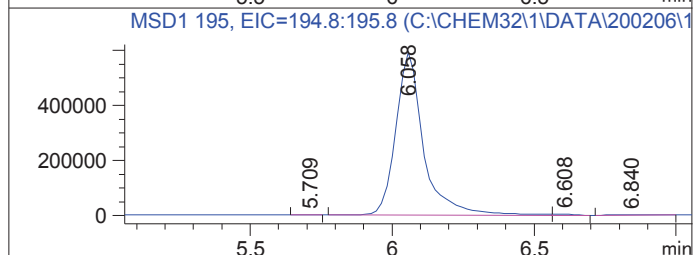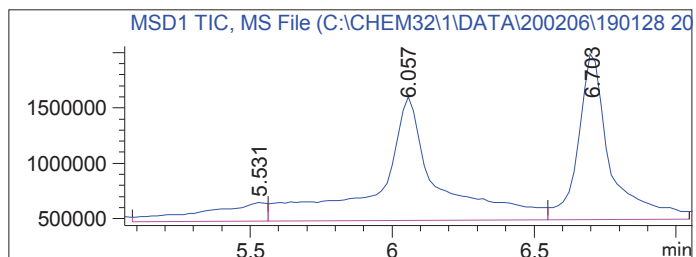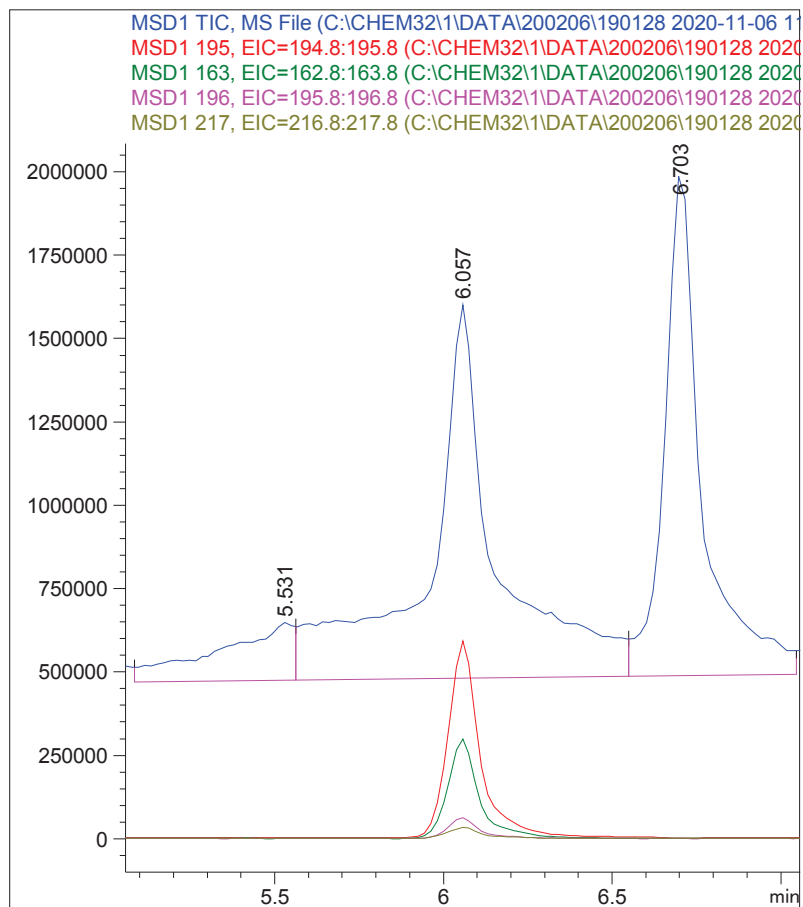

Sample Name: Test_Phthalat_201106

DataPath : C:\CHEM32\1\DATA\200206\190128 2020-11-06 11-24-01\TEST_PHTHALAT_201106.D








DateTime : 11/06/2020 00:09:14 pm

Operator : SYSTEM

Vial : 2

Sample : Test_Phthalat_201106

Retention : 6.703 minutes

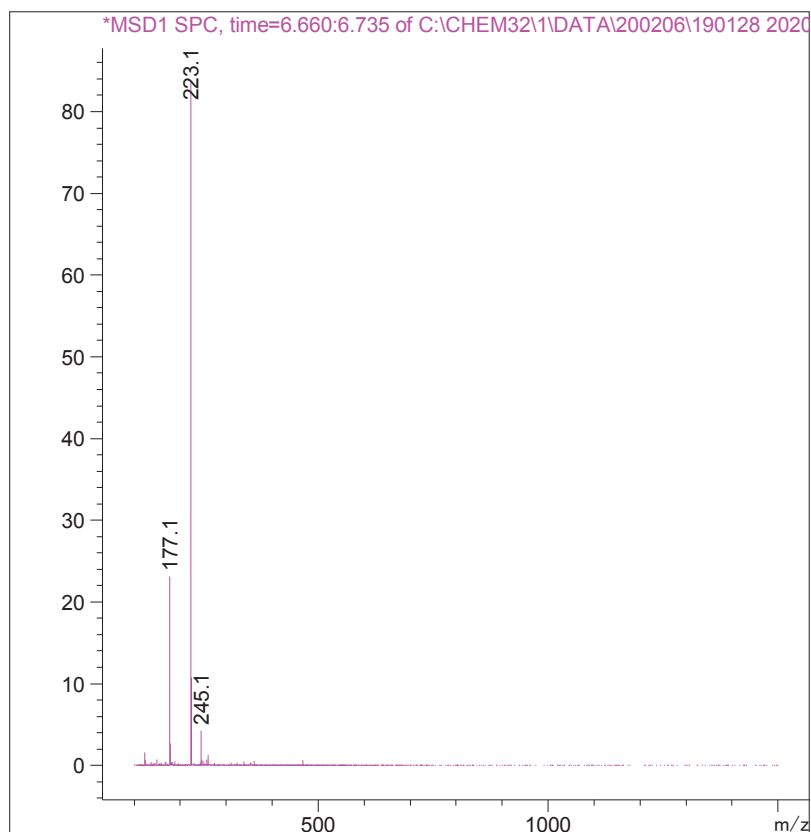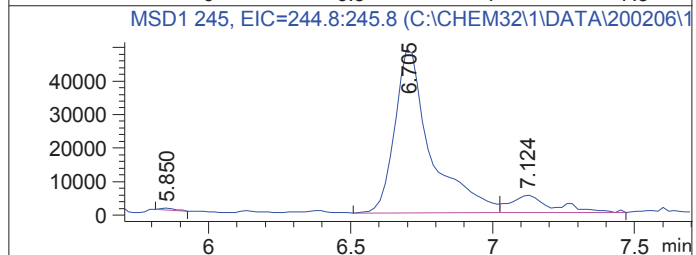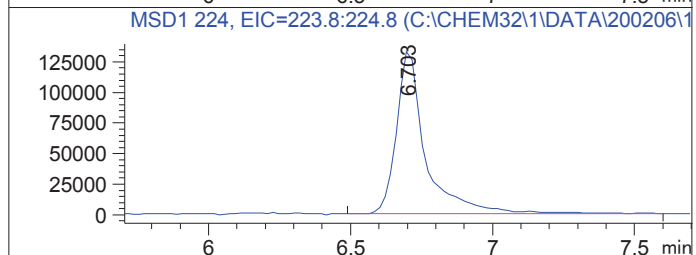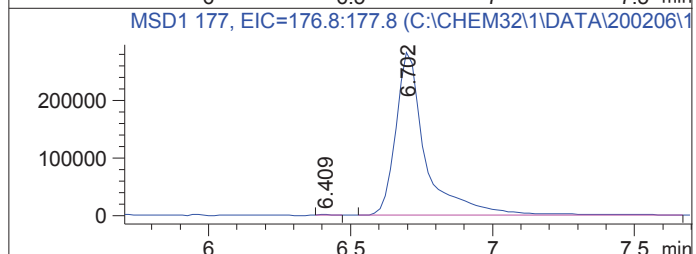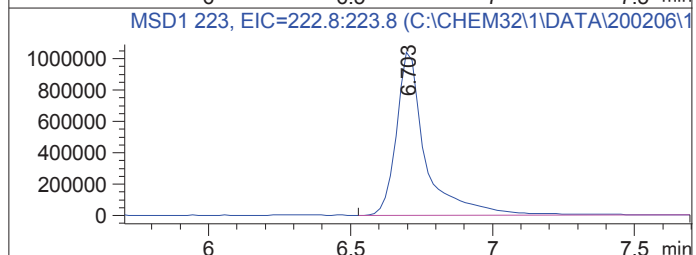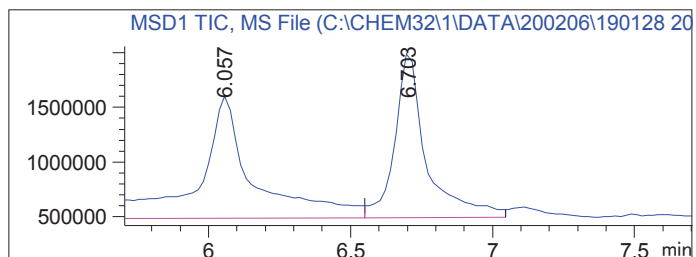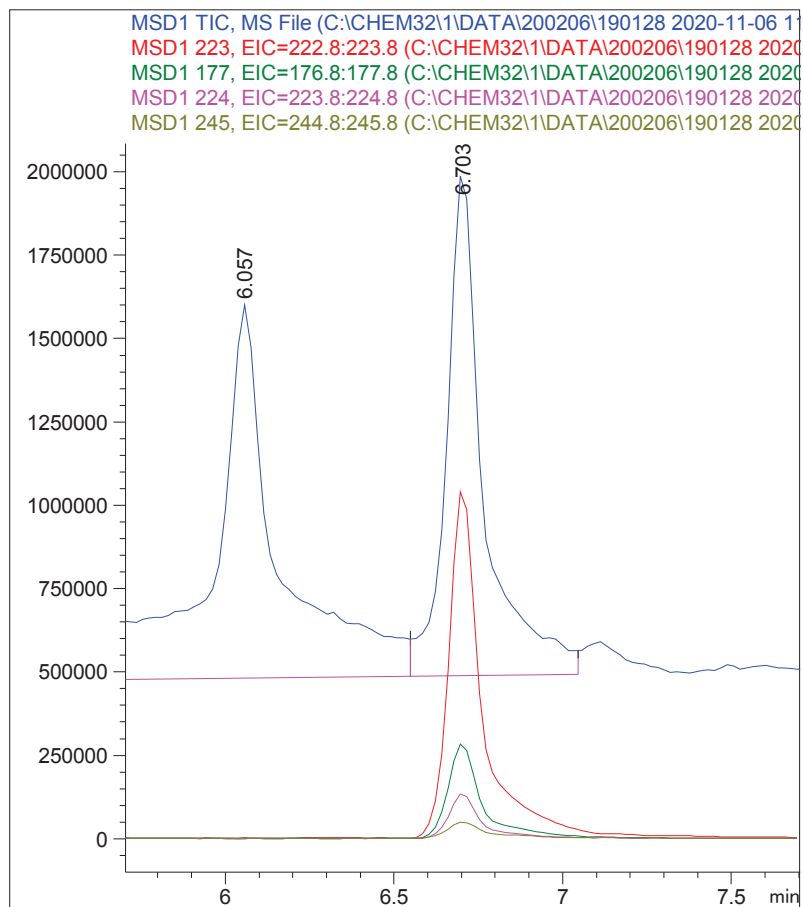

Sample Name: Test_Phthalat_201106

DataPath : C:\CHEM32\1\DATA\200206\190128 2020-11-06 11-24-01\TEST_PHTHALAT_201106.D

DateTime : 11/06/2020 00:09:14 pm

Operator : SYSTEM

Vial : 2

Sample : Test_Phthalat_201106

Retention : 8.356 minutes

