


Sample Name: testmix

```
=====
Acq. Operator   : SYSTEM                      Seq. Line :    1
Acq. Instrument : LCMS 1                     Location  : Vial 3
Injection Date  : 1/10/2013 8:43:41 AM      Inj       :    1
                                           Inj Volume: 1.000 µl
Acq. Method     : C:\CHEM32\1\DATA\DEF_LC 2013-01-10 08-41-51\STANDARD_220NM.M
Last changed    : 1/10/2013 8:41:51 AM by SYSTEM
Analysis Method : C:\CHEM32\1\DATA\DEF_LC 2013-01-10 08-41-51\STANDARD_220NM.M (Sequence
Method)
Last changed    : 1/11/2013 10:50:50 AM by SYSTEM
                 (modified after loading)
Method Info     : Standard ACN:Wasser 20:80 -> 95:5 Flow 0.4 ml/min 220nm
```

Additional Info : Peak(s) manually integrated

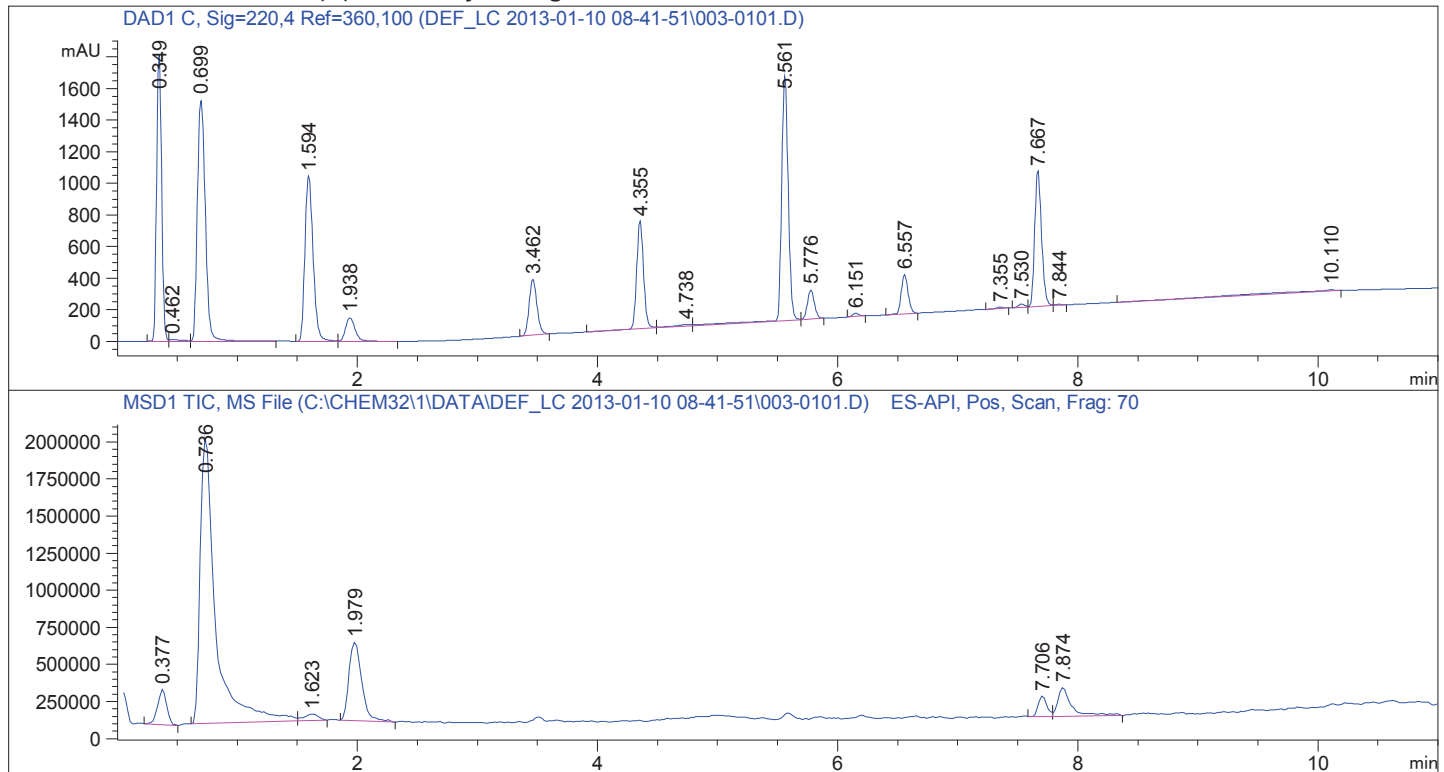

Spectra averaged over upper half of peaks.

Number of ions per peak: 6

Display Time Range(+/- mins): 1.0

Sample Name: testmix

DataPath : C:\CHEM32\1\DATA\DEF\_LC 2013-01-10 08-41-51\003-0101.D










DateTime: 10 Jan 13 8:43 am +0100

Operator : SYSTEM

Vial : 3

Sample : testmix

Retention : 0.377 minutes

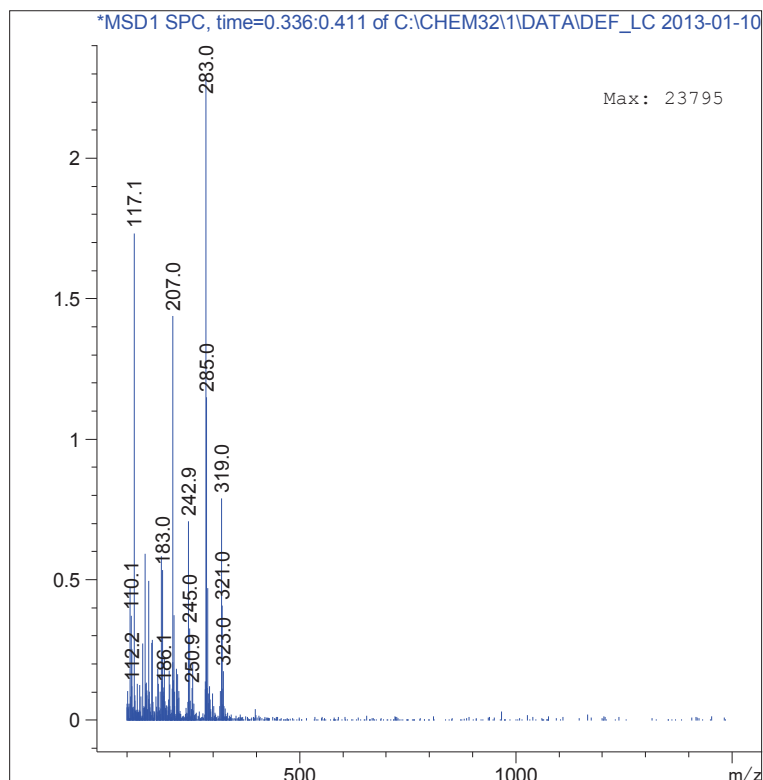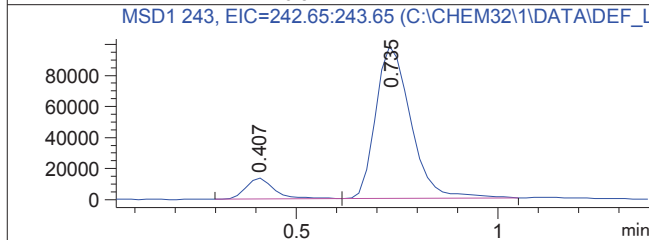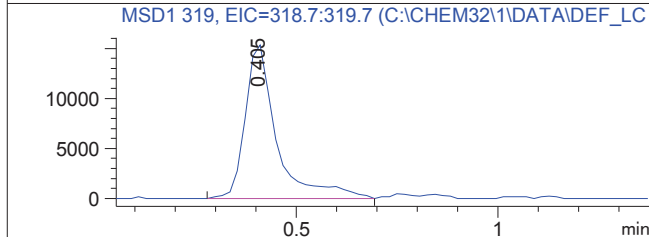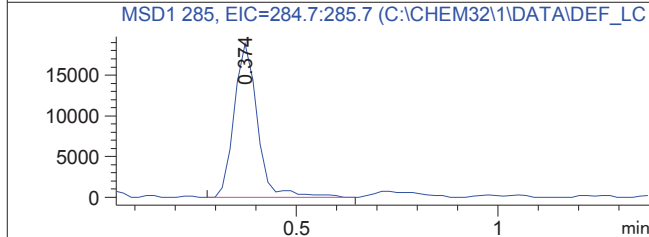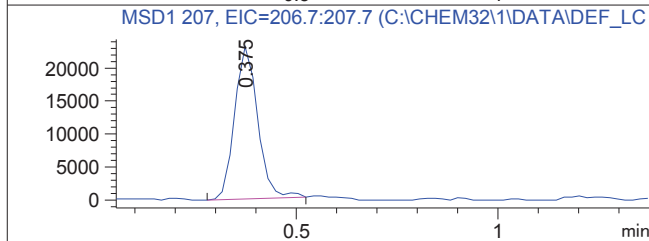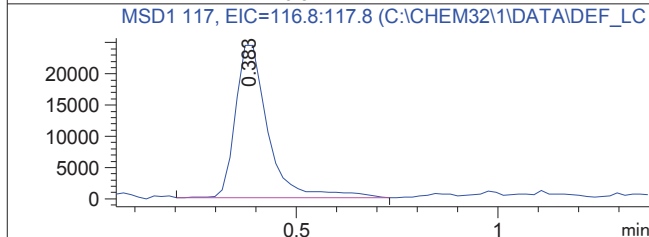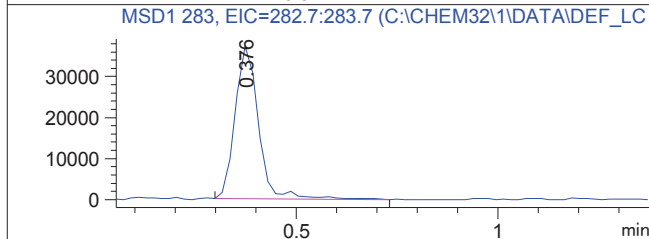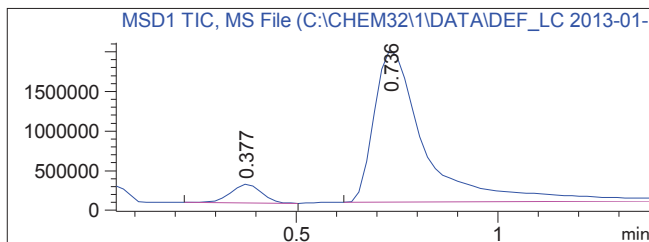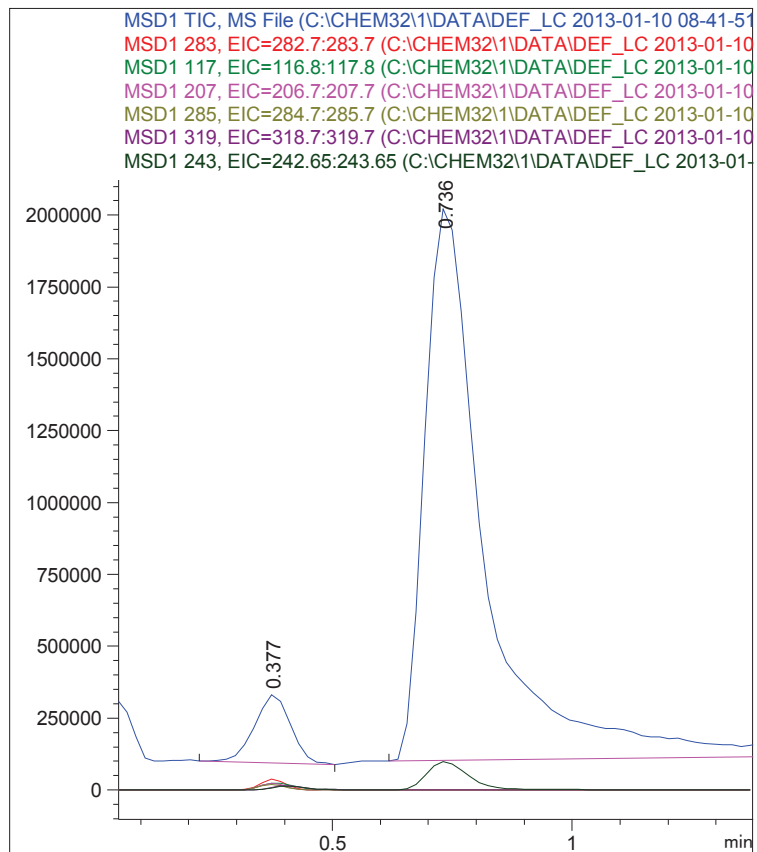

Sample Name: testmix

DataPath : C:\CHEM32\1\DATA\DEF\_LC 2013-01-10 08-41-51\003-0101.D








DateTime: 10 Jan 13 8:43 am +0100

Operator : SYSTEM

Vial : 3

Sample : testmix

Retention : 0.736 minutes

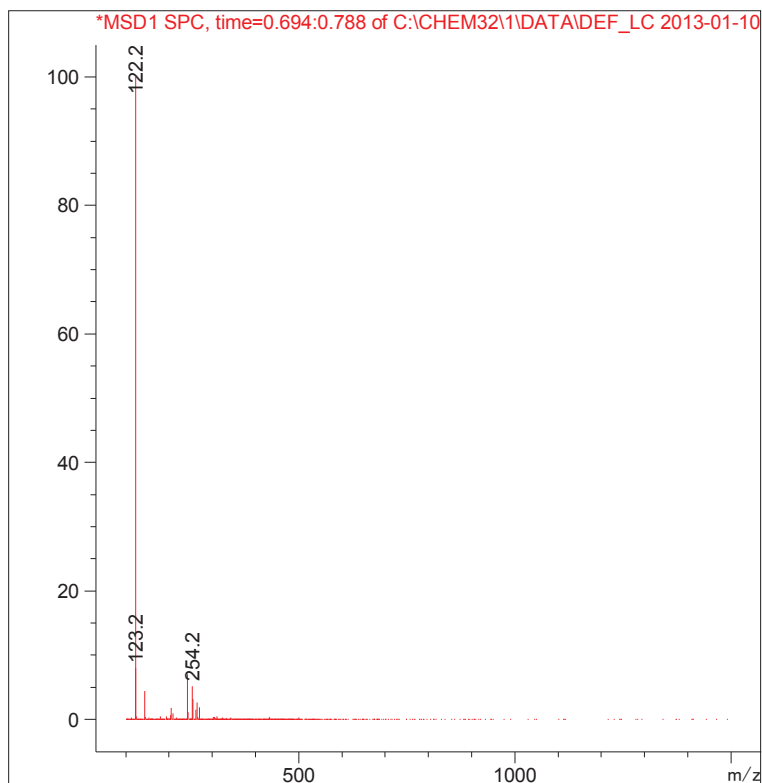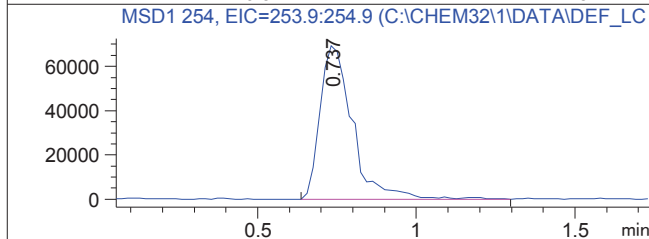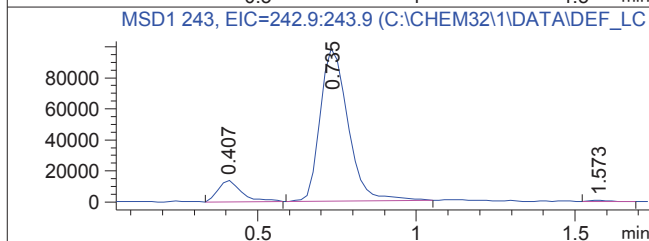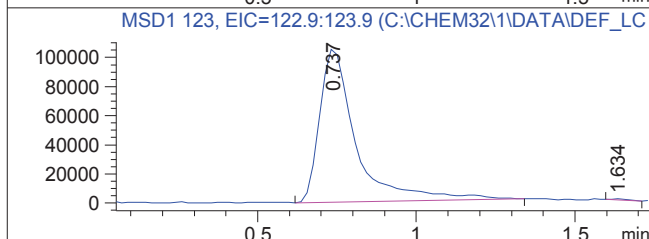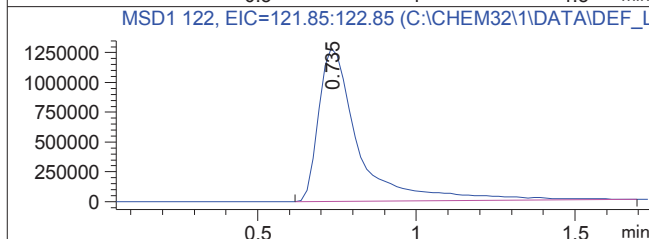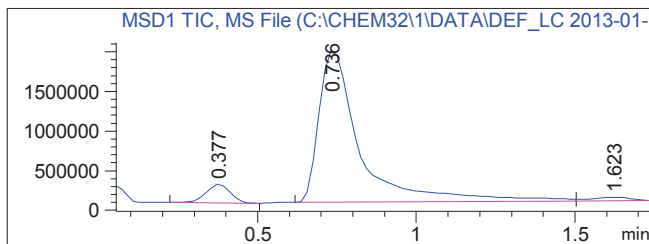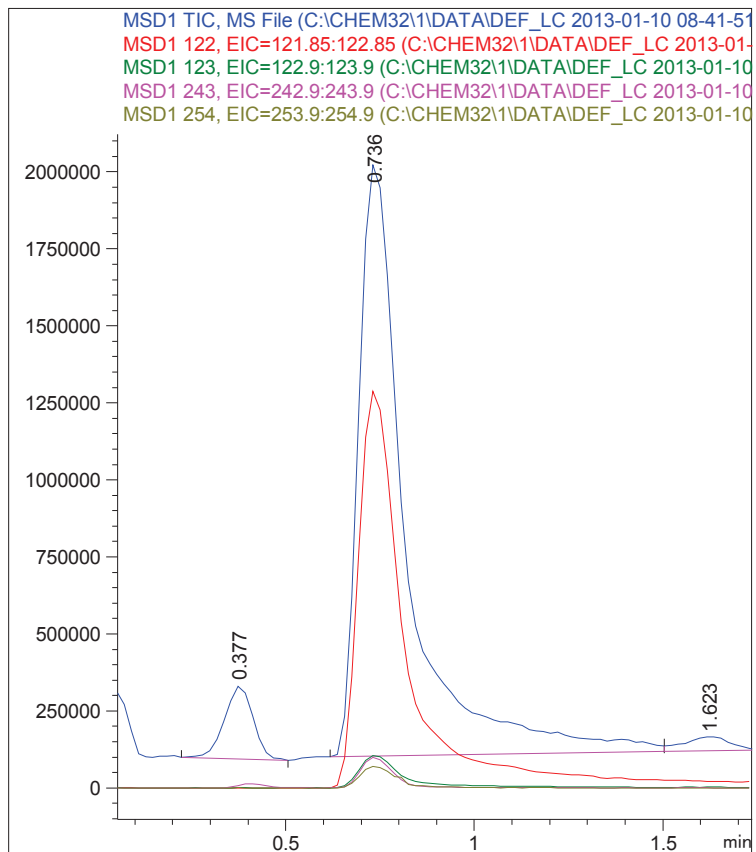

Sample Name: testmix

DataPath : C:\CHEM32\1\DATA\DEF\_LC 2013-01-10 08-41-51\003-0101.D









DateTime: 10 Jan 13 8:43 am +0100

Operator : SYSTEM

Vial : 3

Sample : testmix

Retention : 1.623 minutes

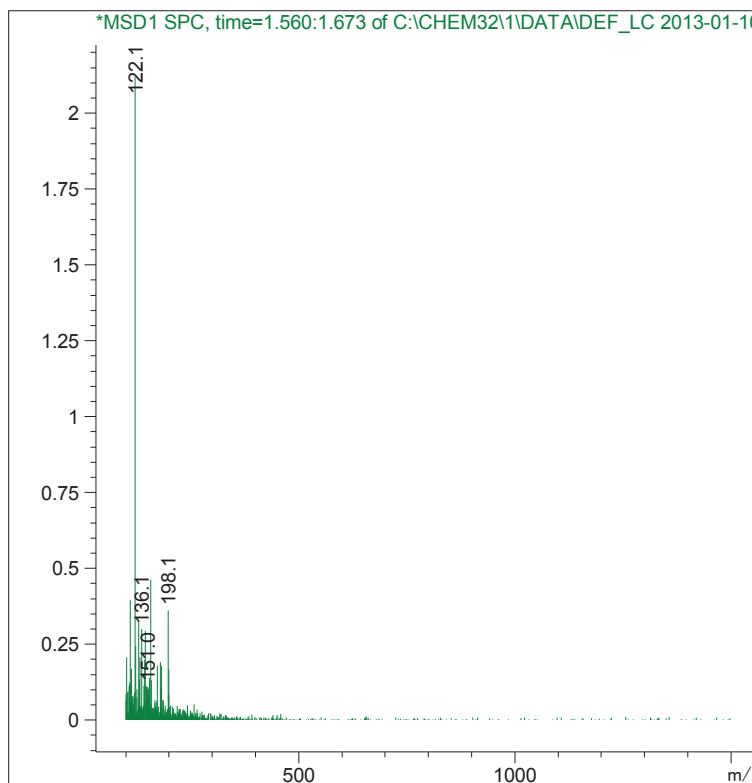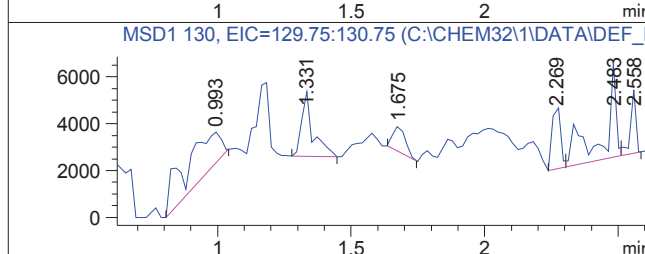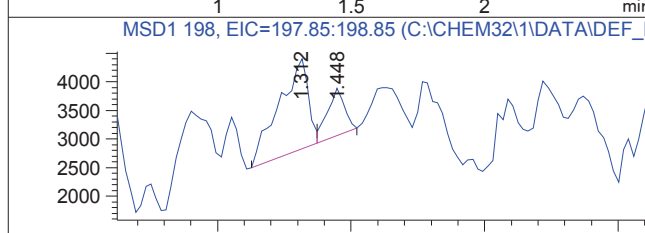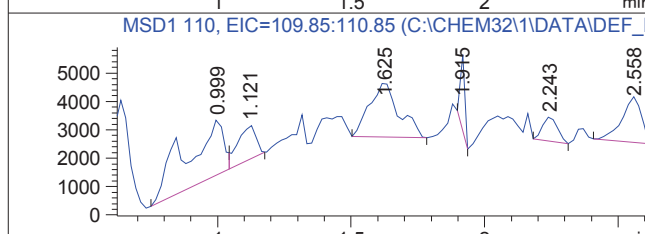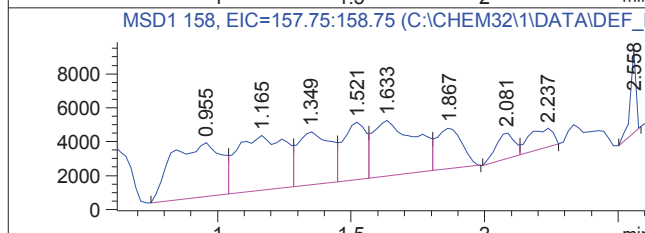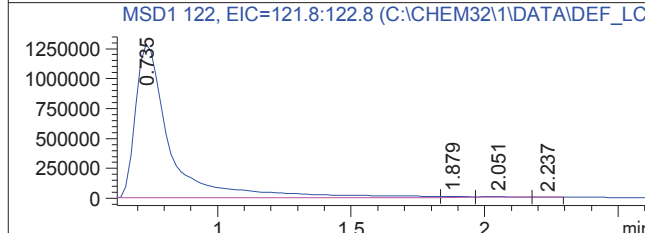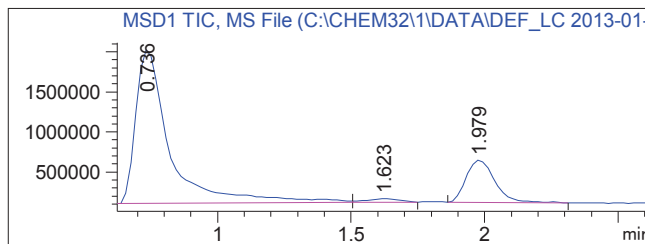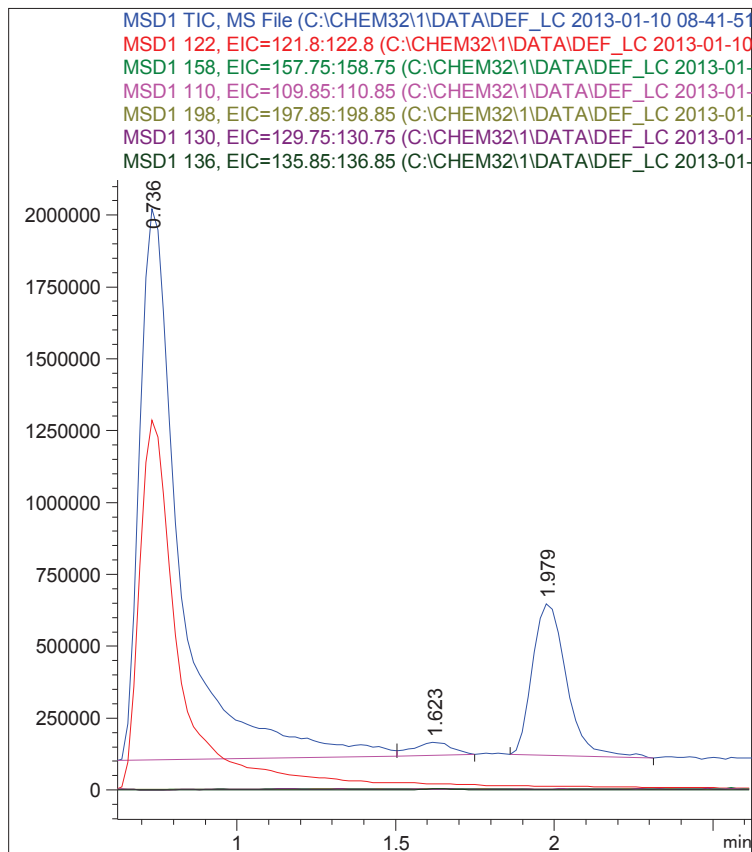

Sample Name: testmix

DataPath : C:\CHEM32\1\DATA\DEF\_LC 2013-01-10 08-41-51\003-0101.D




DateTime: 10 Jan 13 8:43 am +0100

Operator : SYSTEM

Vial : 3

Sample : testmix

Retention : 1.979 minutes

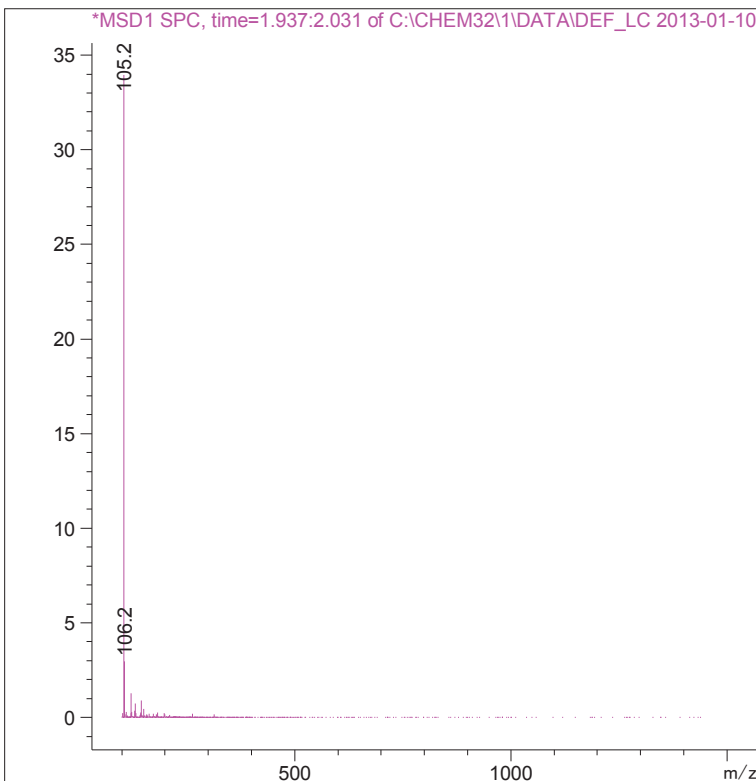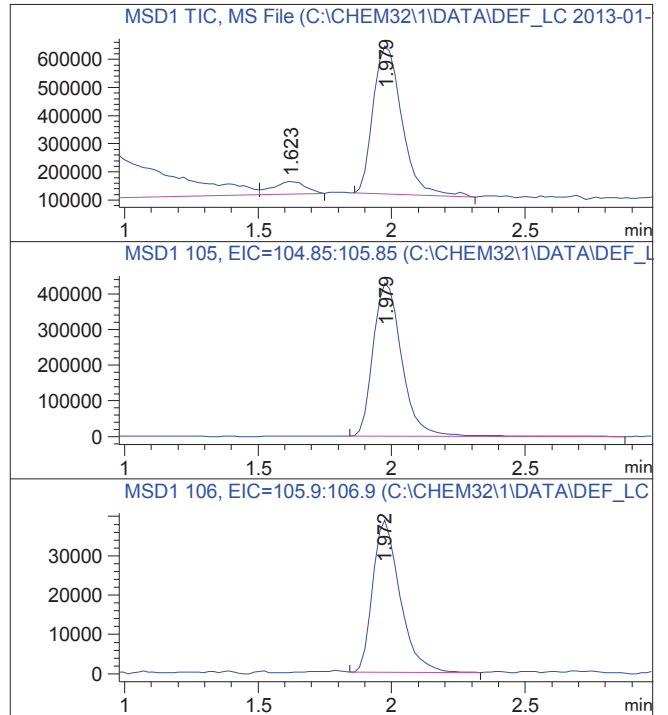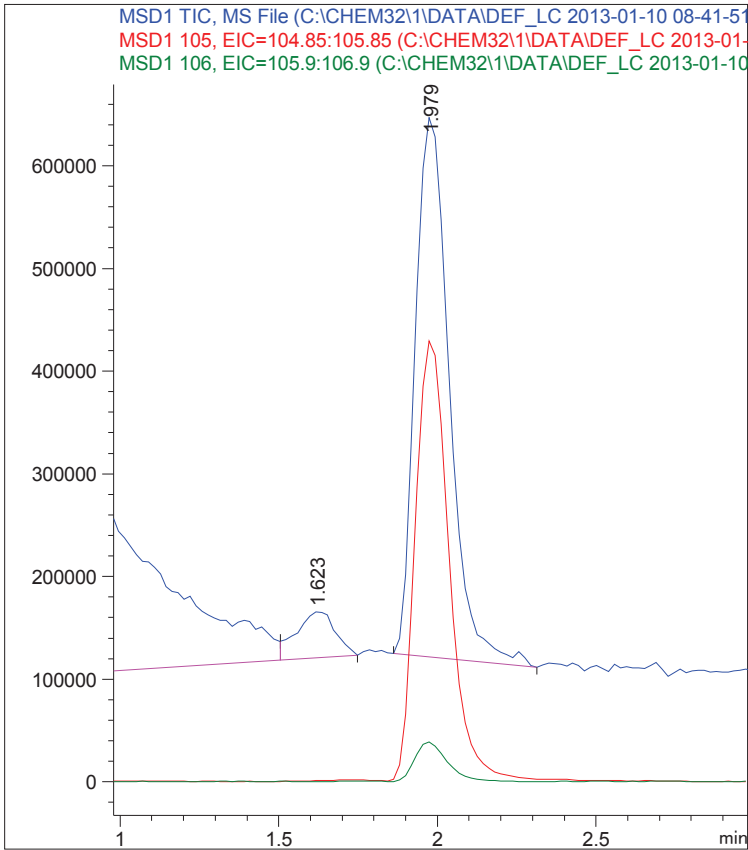

Sample Name: testmix

DataPath : C:\CHEM32\1\DATA\DEF\_LC 2013-01-10 08-41-51\003-0101.D









DateTime: 10 Jan 13 8:43 am +0100

Operator : SYSTEM

Vial : 3

Sample : testmix

Retention : 7.706 minutes

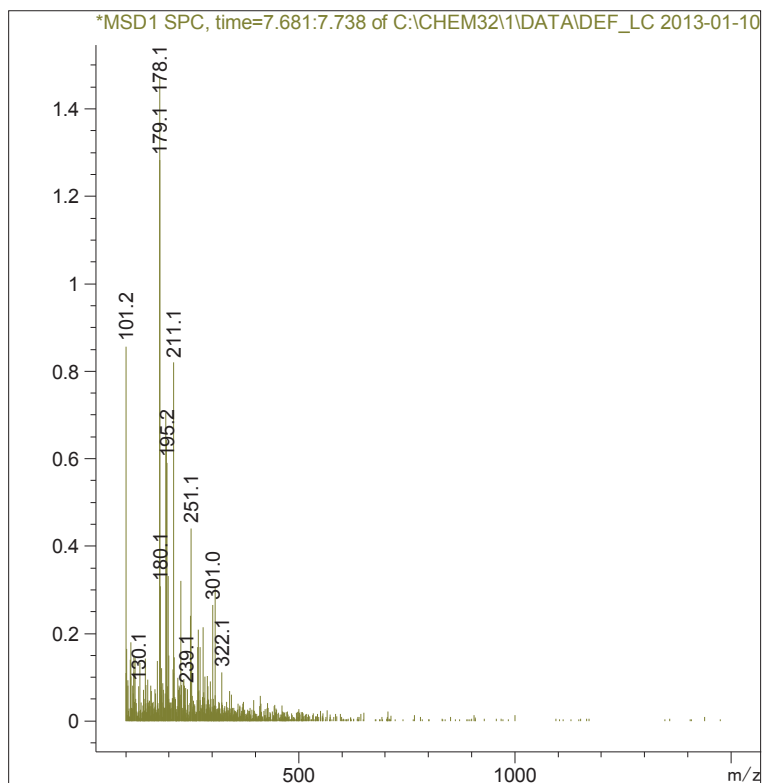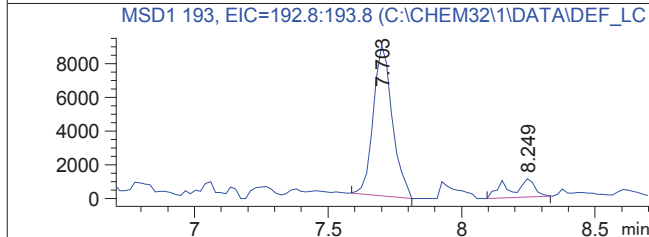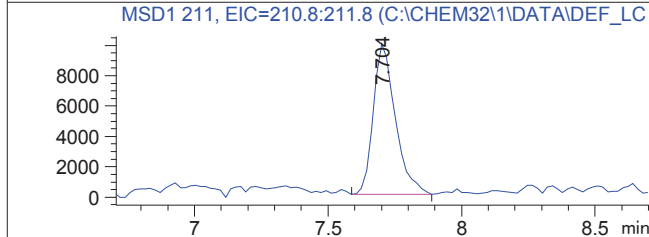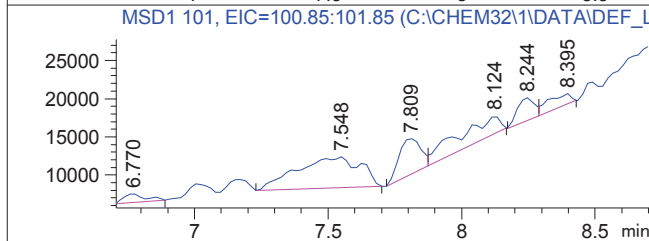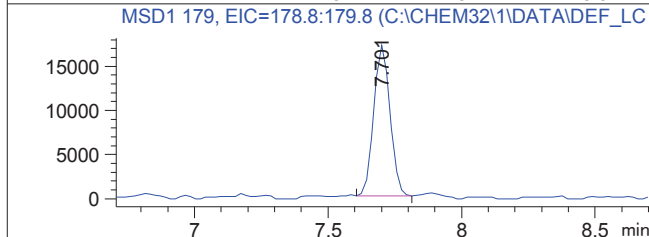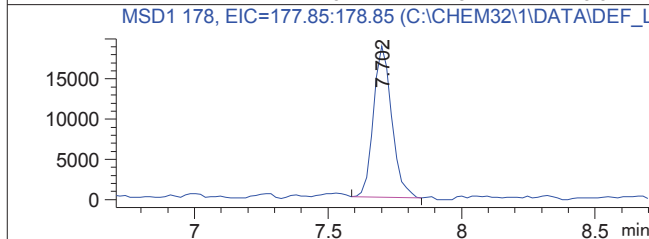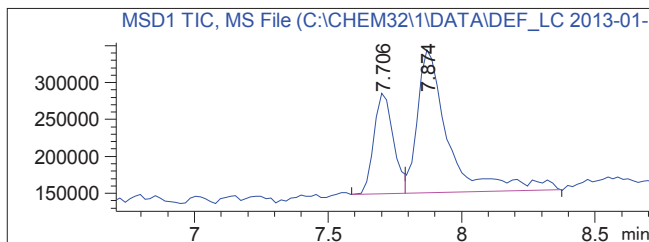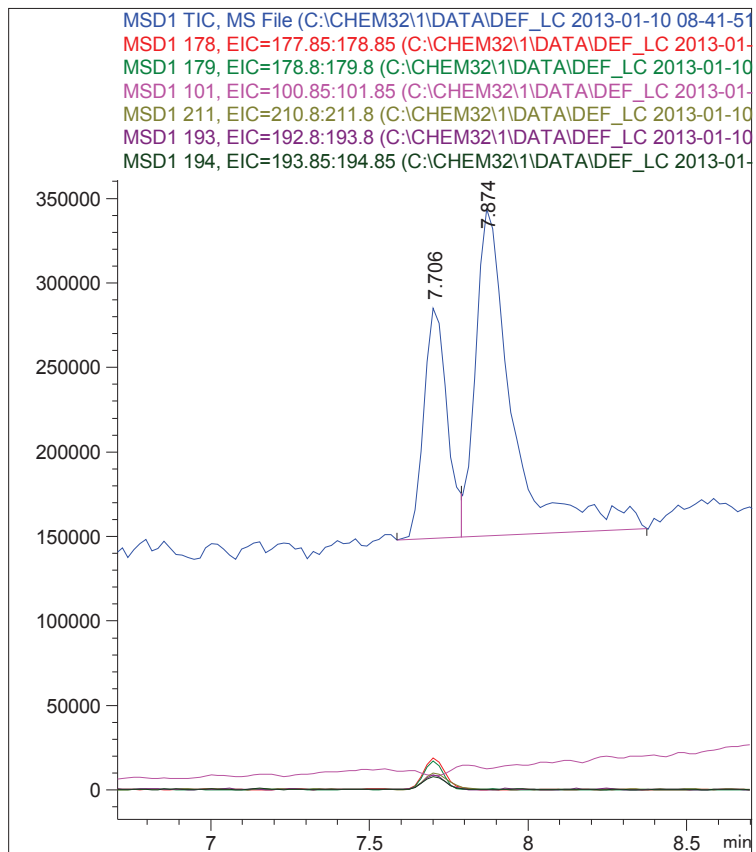

Sample Name: testmix

DataPath : C:\CHEM32\1\DATA\DEF\_LC 2013-01-10 08-41-51\003-0101.D

DateTime: 10 Jan 13 8:43 am +0100

Operator : SYSTEM

Vial : 3

Sample : testmix

Retention : 7.874 minutes

