


```
=====
Acq. Operator   : SYSTEM
Acq. Instrument : PrepLC                               Location : Vial 1
Injection Date  : 4/22/2013 2:08:44 PM
Method         : C:\CHEM32\1\METHODS\STANDARD_PREP.M
Last changed   : 4/22/2013 2:04:08 PM by SYSTEM
Method Info    : ACN:Wasser 80:20 Flow 20ml/min 250nm
=====
```

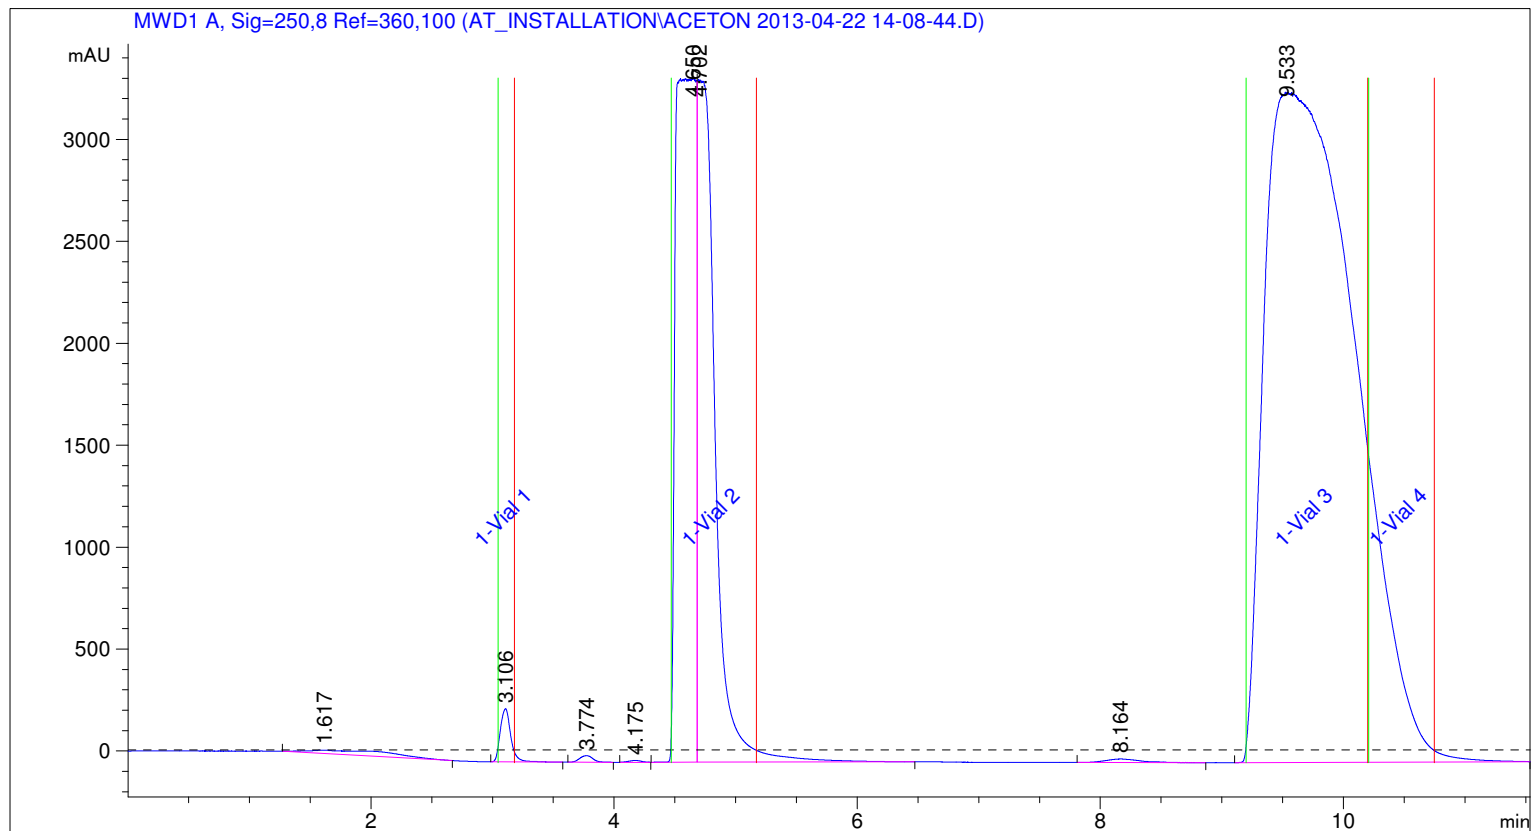

=====
 Fraction Information
 =====

Fraction collection peak controlled
 Maximum peak duration 1 min.
 Fractions are collected, when at least one peak detector detects a peak

Frac #	Well #	Location	Volume [µl]	BeginTime [min]	EndTime [min]	Reason	Mass
1	1	1-Vial 1	0.00	3.0469	3.1804	MWD1	
2	1	1-Vial 2	0.00	4.4708	5.1710	MWD1	
3	1	1-Vial 3	0.00	9.2008	10.2004	MWD1	
4	1	1-Vial 4	0.00	10.2081	10.7471	MWD1	

=====
 Area Percent Report
 =====

```
Sorted By       : Signal
Multiplier     : 1.0000
Dilution       : 1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Signal 1: MWD1 A, Sig=250,8 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	1.617	BB	0.7529	1012.82904	15.94899	0.4099
2	3.106	BB	0.0946	1575.50781	260.33182	0.6375
3	3.774	BB	0.1212	241.78374	32.34799	0.0978
4	4.175	BB	0.1163	63.71729	8.61117	0.0258
5	4.650	BV	0.1393	3.82859e4	3351.90259	15.4928
6	4.702	VB	0.1246	3.39721e4	3342.84839	13.7471
7	8.164	BB	0.2533	340.30804	17.31194	0.1377
8	9.533	BBA	0.6202	1.71629e5	3281.67480	69.4514

Totals : 2.47122e5 1.03110e4

=====
*** End of Report ***