


```

=====
Acq. Operator   : SYSTEM
Acq. Instrument : PrepLC                               Location : Vial 1
Injection Date  : 4/25/2013 2:19:38 PM
Method         : C:\CHEM32\1\METHODS\STANDARD_PREP.M
Last changed   : 4/25/2013 2:01:32 PM by SYSTEM
Method Info    : ACN:Wasser 80:20 Flow 20ml/min 254nm
  
```

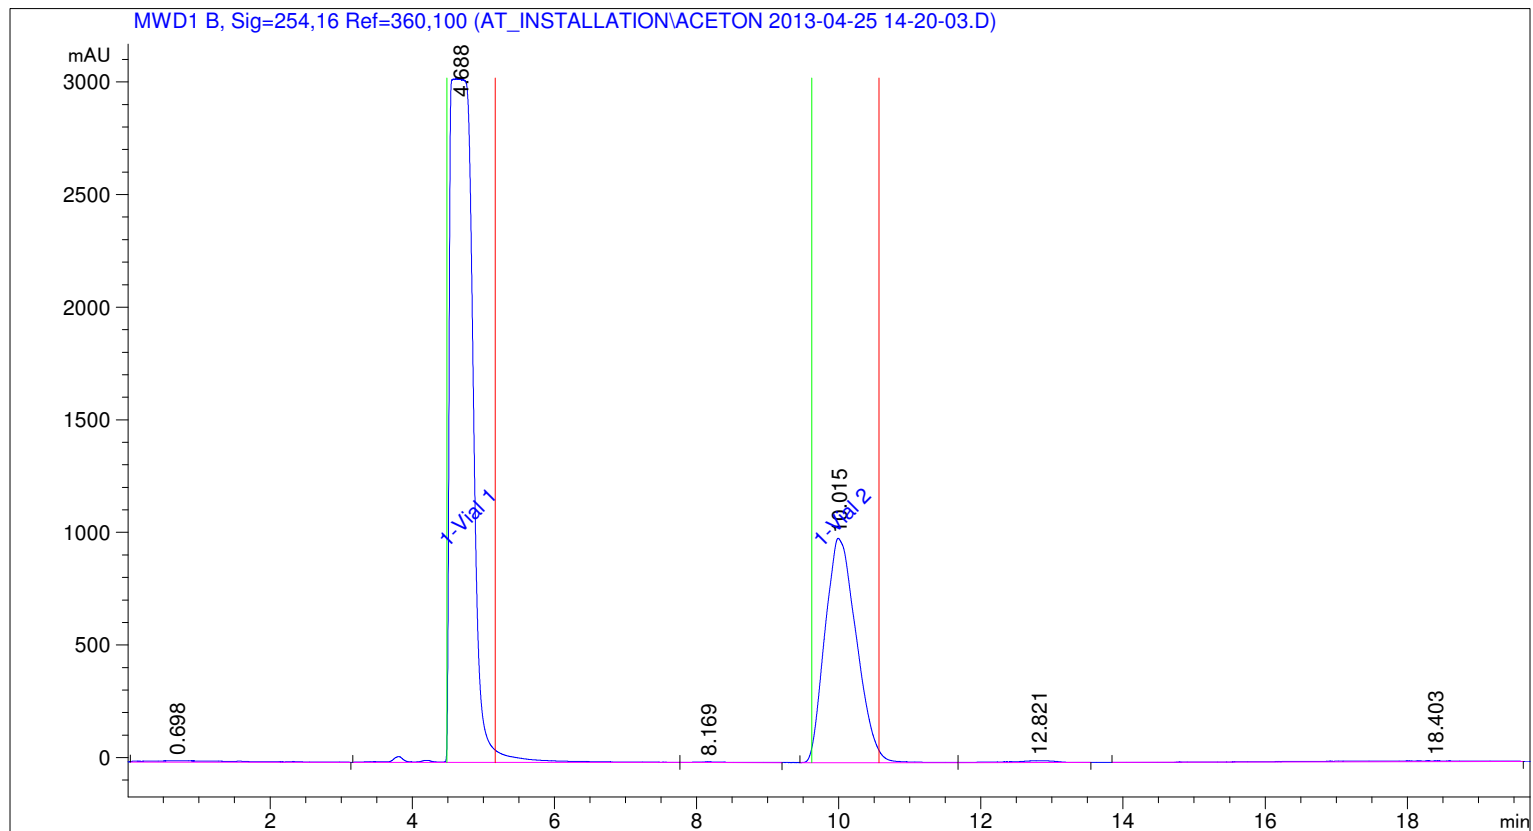

Fraction Information

```

=====
Fraction collection peak controlled
Maximum peak duration 1 min.
Fractions are collected, when at least one peak detector detects a peak
  
```

Frac #	Well #	Location	Volume [µl]	BeginTime [min]	EndTime [min]	Reason	Mass
1	1	1-Vial 1	0.00	4.4900	5.1656	MWD1	
2	1	1-Vial 2	0.00	9.6200	10.5679	MWD1	

Area Percent Report

```

=====
Sorted By      : Signal
Multiplier    : 1.0000
Dilution      : 1.0000
Use Multiplier & Dilution Factor with ISTDs
  
```

Signal 1: MWD1 B, Sig=254,16 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	0.698	BB	1.3481	581.75226	5.63648	0.5813
2	4.688	BV	0.3549	6.78481e4	3057.18604	67.8010
3	8.169	VB	0.5068	94.20632	2.78362	0.0941
4	10.015	BV	0.5029	3.05735e4	993.86877	30.5523
5	12.821	VB	0.6802	360.90787	7.85338	0.3607
6	18.403	BBA	2.6182	610.95898	2.79062	0.6105

Totals : 1.00069e5 4070.11891

=====
*** End of Report ***