


Sample Name: Aceton

```

=====
Acq. Operator   : SYSTEM
Acq. Instrument : PrepLC                               Location : Vial 1
Injection Date  : 4/25/2013 2:19:38 PM
Acq. Method     : C:\CHEM32\1\METHODS\STANDARD_PREP.M
Last changed    : 4/25/2013 2:01:32 PM by SYSTEM
Analysis Method : C:\CHEM32\1\METHODS\STANDARD_PREP.M
Last changed    : 4/26/2013 10:29:15 AM by SYSTEM
                  (modified after loading)
Method Info     : ACN:Wasser 80:20 Flow 20ml/min 254nm
    
```

Additional Info : Peak(s) manually integrated

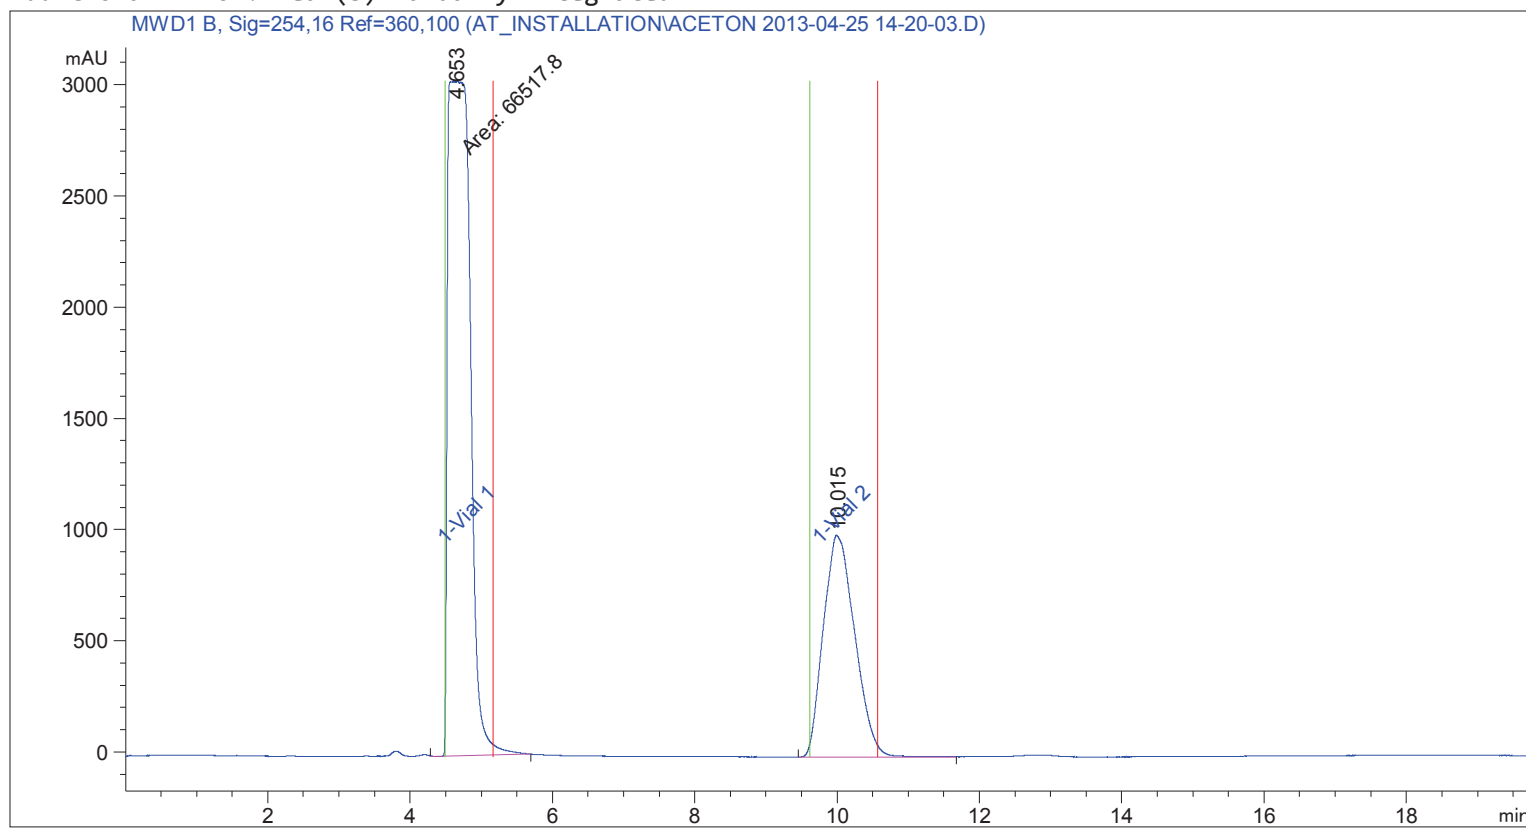

Fraction Information

```

=====
Fraction collection peak controlled
Maximum peak duration 1 min.
Fractions are collected, when at least one peak detector detects a peak
    
```

Frac #	Well #	Location	Volume [µl]	BeginTime [min]	EndTime [min]	Reason	Mass
1	1	1-Vial 1	0.00	4.4900	5.1656	MWD1	
2	1	1-Vial 2	0.00	9.6200	10.5679	MWD1	

Sample Name: Aceton

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 B, Sig=254,16 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	4.653	MM	0.3655	6.65178e4	3033.03906	68.5106
2	10.015	BV	0.5029	3.05735e4	993.86877	31.4894

Totals : 9.70912e4 4026.90784

=====
*** End of Report ***